

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027510.D
 Acq On : 25 Aug 2022 21:56
 Operator : SY/MD
 Sample : N4367-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E82

Quant Time: Aug 26 02:02:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 26 01:50:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	130663	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	120798	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52759	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	33886	3.644	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.564	69	30683	4.508	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.105	63	59387	2.739	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.800%#
20) 2-Butanone-d5	3.905	46	31797	27.475	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	54.960%
24) Chloroform-d	4.349	84	70507	3.792	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.800%
26) 1,2-Dichloroethane-d4	5.034	65	33261	4.135	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
32) Benzene-d6	5.050	84	137082	4.097	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	6.069	67	41354	4.251	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.000%
41) Toluene-d8	7.317	98	111713	3.698	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.000%
43) trans-1,3-Dichloroprop...	7.625	79	12382	3.717	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	8.091	63	44608	40.686	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.380%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26461	4.271	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	35699	4.565	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds						
					Qvalue	
30) Cyclohexane	4.674	56	4507	0.317	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027510.D
Acq On : 25 Aug 2022 21:56
Operator : SY/MD
Sample : N4367-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E82

Quant Time: Aug 26 02:02:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 26 01:50:00 2022
Response via : Initial Calibration

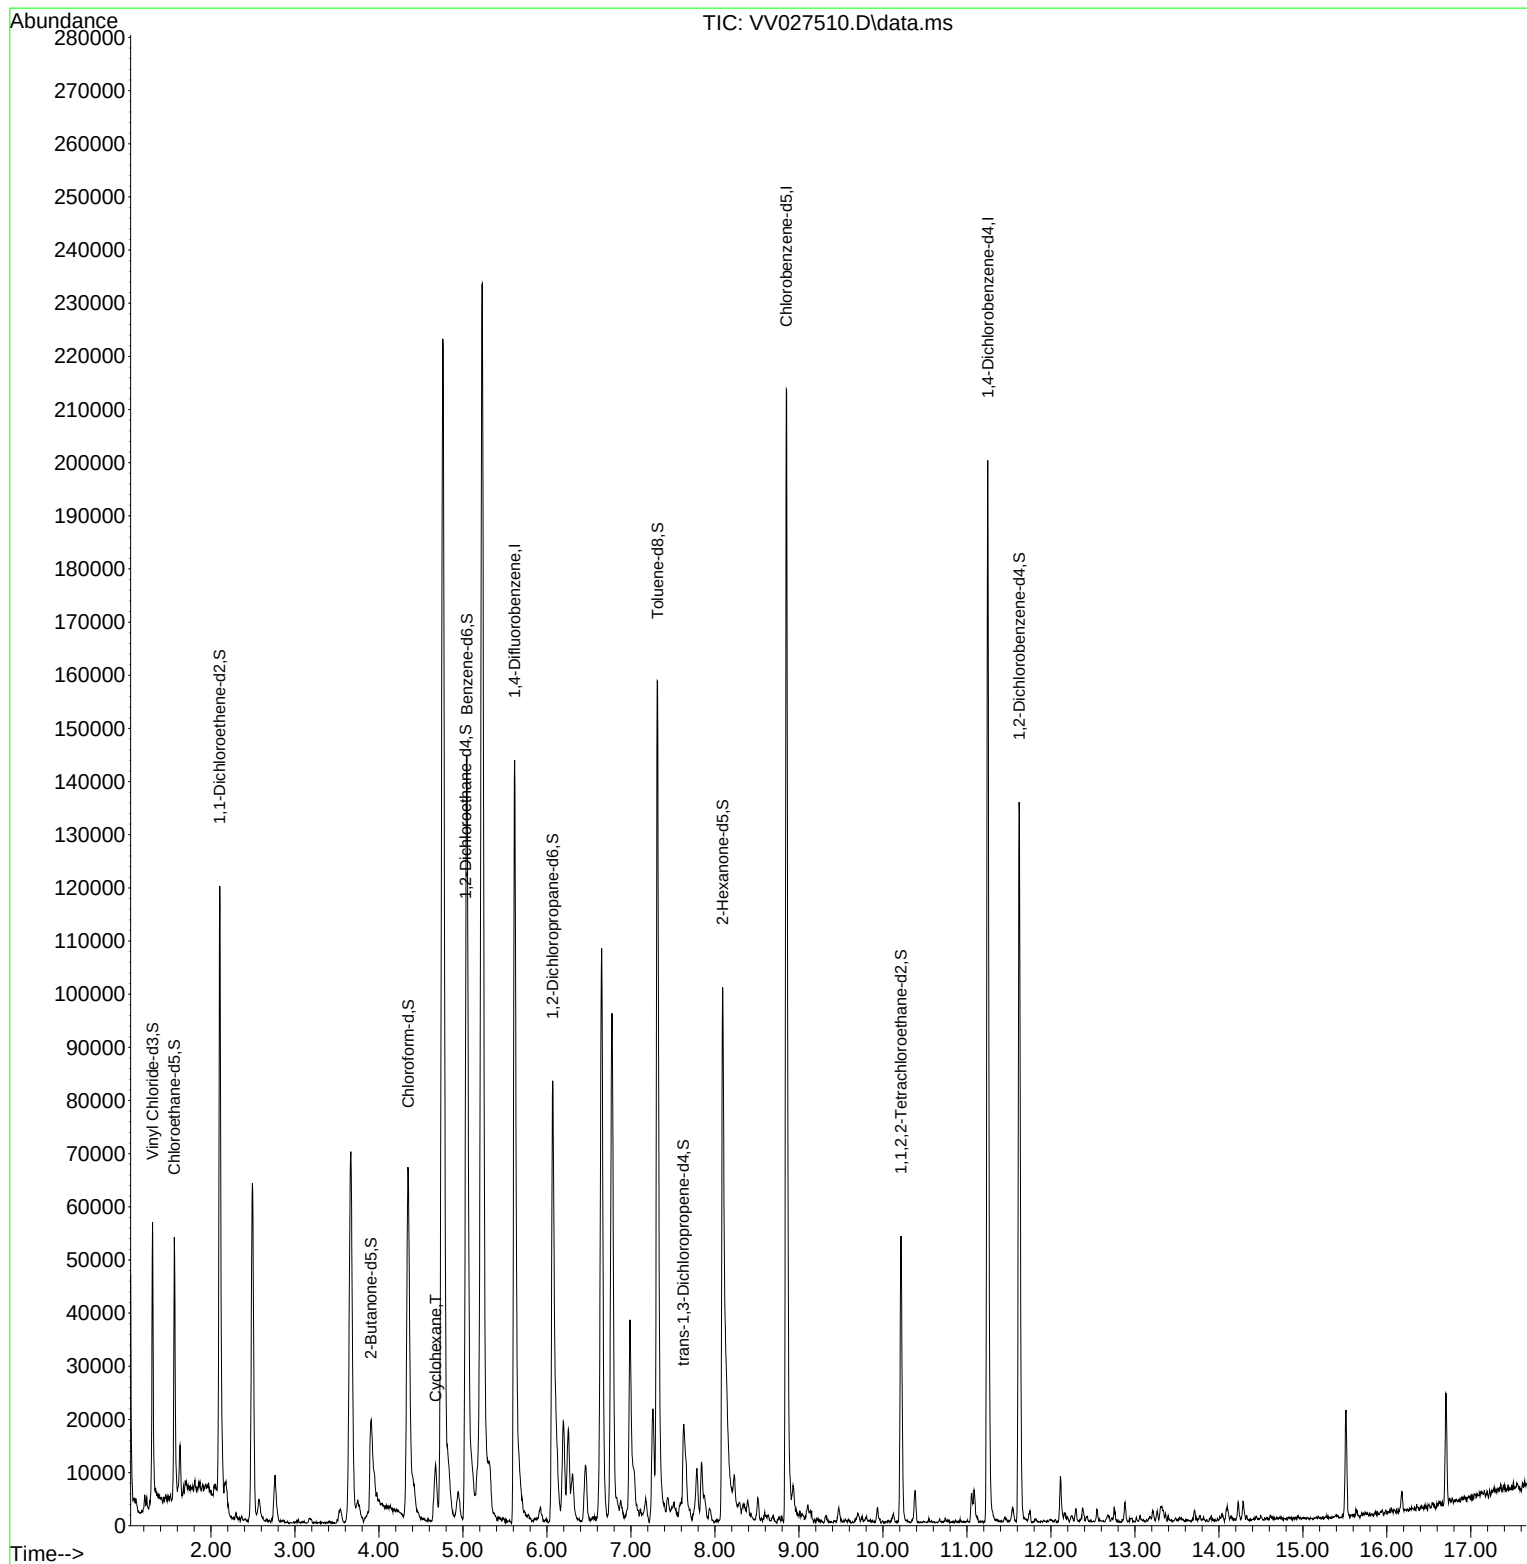

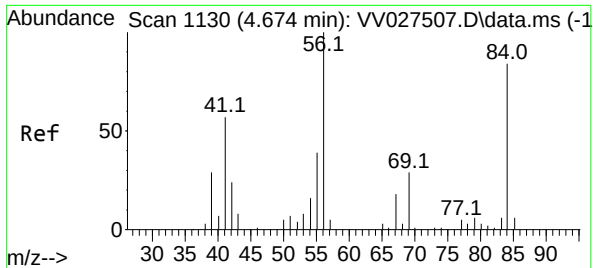

#30
Cyclohexane
Concen: 0.317 ug/L
RT: 4.674 min Scan# 11
Delta R.T. -0.000 min
Lab File: VV027510.D
Acq: 25 Aug 2022 21:56

Instrument :
MSVOA_V
ClientSampleId :
F5E82

Tgt Ion: 56	Resp:	4507
Ion	Ratio	Lower Upper
56	100	
69	35.9	25.4 38.0
84	100.4	69.7 104.5

