

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027519.D
 Acq On : 26 Aug 2022 01:37
 Operator : SY/MD
 Sample : N4367-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F24

Quant Time: Aug 26 02:03:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Aug 26 01:50:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	127761	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	125321	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54656	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	32691	3.595	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	72.000%	
7) Chloroethane-d5	1.564	69	30568	4.593	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.105	63	58377	2.753	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.000%#	
20) 2-Butanone-d5	3.899	46	32242	28.493	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	56.980%	
24) Chloroform-d	4.349	84	69027	3.797	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	76.000%	
26) 1,2-Dichloroethane-d4	5.031	65	32899	4.183	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.600%	
32) Benzene-d6	5.050	84	120542	3.473	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	69.400%#	
36) 1,2-Dichloropropane-d6	6.069	67	37661	3.732	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	74.600%	
41) Toluene-d8	7.317	98	95723	3.054	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	61.000%#	
43) trans-1,3-Dichloroprop...	7.629	79	9125	2.641	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	52.800%#	
46) 2-Hexanone-d5	8.092	63	38856	34.160	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	68.320%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24210	3.767	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	75.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	32613	4.025	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	80.600%	
Target Compounds					Qvalue	
25) Chloroform	4.375	83	20429	0.911	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027519.D
Acq On : 26 Aug 2022 01:37
Operator : SY/MD
Sample : N4367-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F24

Quant Time: Aug 26 02:03:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Aug 26 01:50:00 2022
Response via : Initial Calibration

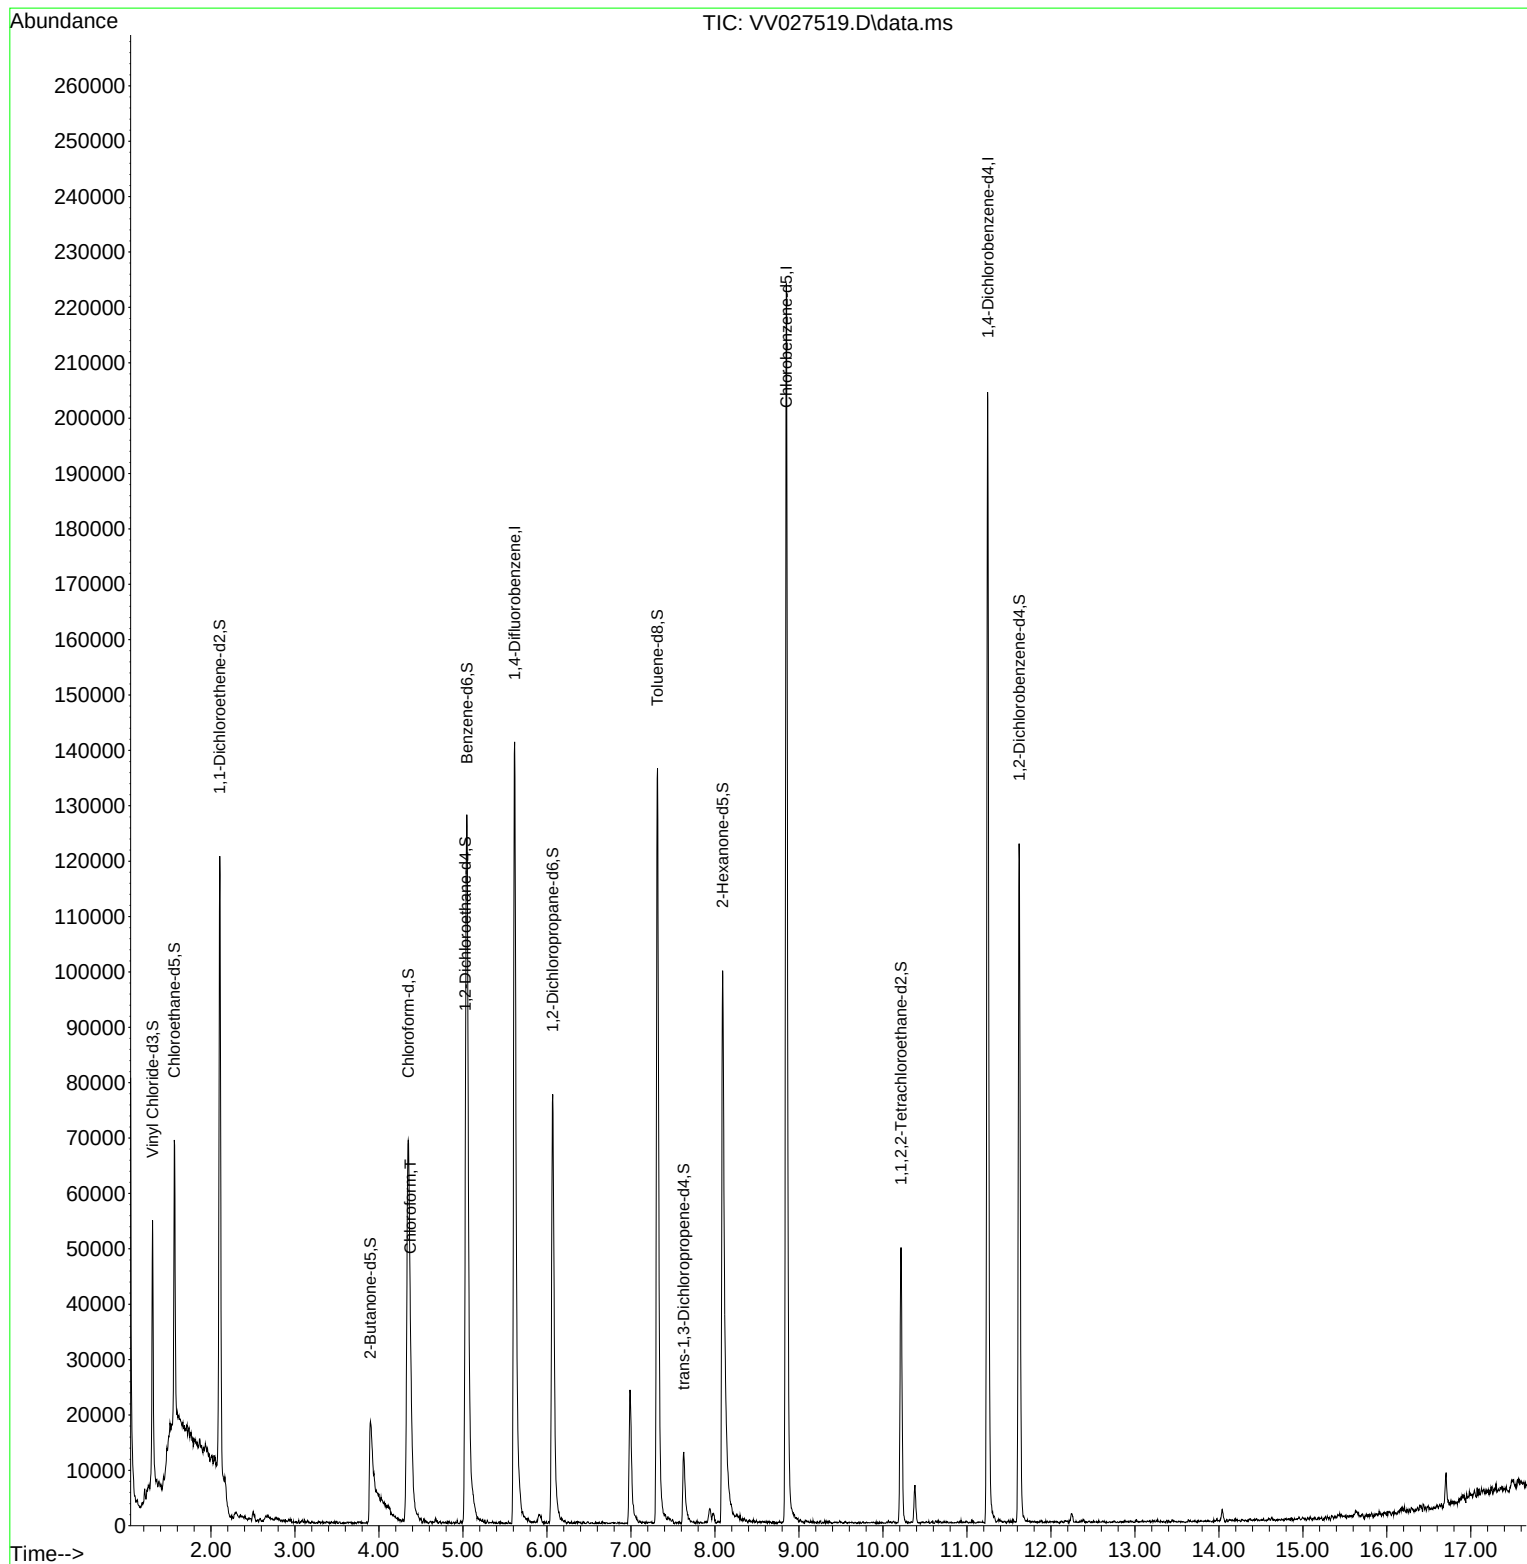

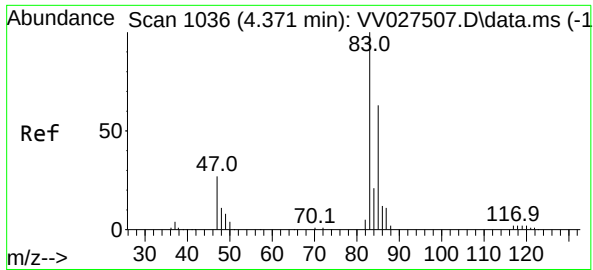

#25
 Chloroform
 Concen: 0.911 ug/L
 RT: 4.375 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV027519.D
 Acq: 26 Aug 2022 01:37

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F24

Tgt Ion: 83 Resp: 20429
 Ion Ratio Lower Upper
 83 100
 85 64.0 43.3 80.5

