

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027495.D
 Acq On : 25 Aug 2022 09:49
 Operator : SY/MD
 Sample : VV0825WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	39	rVB	5257	5729	1.49%	0.184%
2	1.304	73	82	91	rBV	49128	55154	14.38%	1.772%
3	1.564	156	163	173	rBV	59494	68091	17.75%	2.188%
4	2.105	320	331	341	rBV	125124	182638	47.60%	5.868%
5	2.503	446	455	465	rVB3	4760	7050	1.84%	0.227%
6	3.889	869	886	911	rBV3	21291	74093	19.31%	2.380%
7	4.342	1011	1027	1062	rVB	69625	190014	49.52%	6.105%
8	5.043	1229	1245	1270	rBV2	148332	383674	100.00%	12.327%
9	5.612	1410	1422	1450	rBV2	134366	296709	77.33%	9.533%
10	6.066	1551	1563	1586	rBV	86046	189274	49.33%	6.081%
11	6.985	1836	1849	1868	rBV	29673	60886	15.87%	1.956%
12	7.313	1938	1951	1973	rBV	157622	298562	77.82%	9.592%
13	7.622	2039	2047	2066	rBV2	17188	34628	9.03%	1.113%
14	8.091	2182	2193	2228	rBV	88765	247985	64.63%	7.967%
15	8.850	2416	2429	2451	rBV	210704	361475	94.21%	11.614%
16	10.214	2843	2853	2866	rBV	52753	86420	22.52%	2.777%
17	11.246	3163	3174	3196	rBV	197561	318456	83.00%	10.231%
18	11.622	3279	3291	3310	rBV	141162	228190	59.47%	7.331%
19	13.509	3870	3878	3888	rBV2	6736	10563	2.75%	0.339%
20	13.747	3943	3952	3961	rVB5	3023	4666	1.22%	0.150%
21	16.471	4796	4799	4803	rBV	13788	8261	2.15%	0.265%




Sum of corrected areas: 3112518

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027495.D
Acq On : 25 Aug 2022 09:49
Operator : SY/MD
Sample : VV0825WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

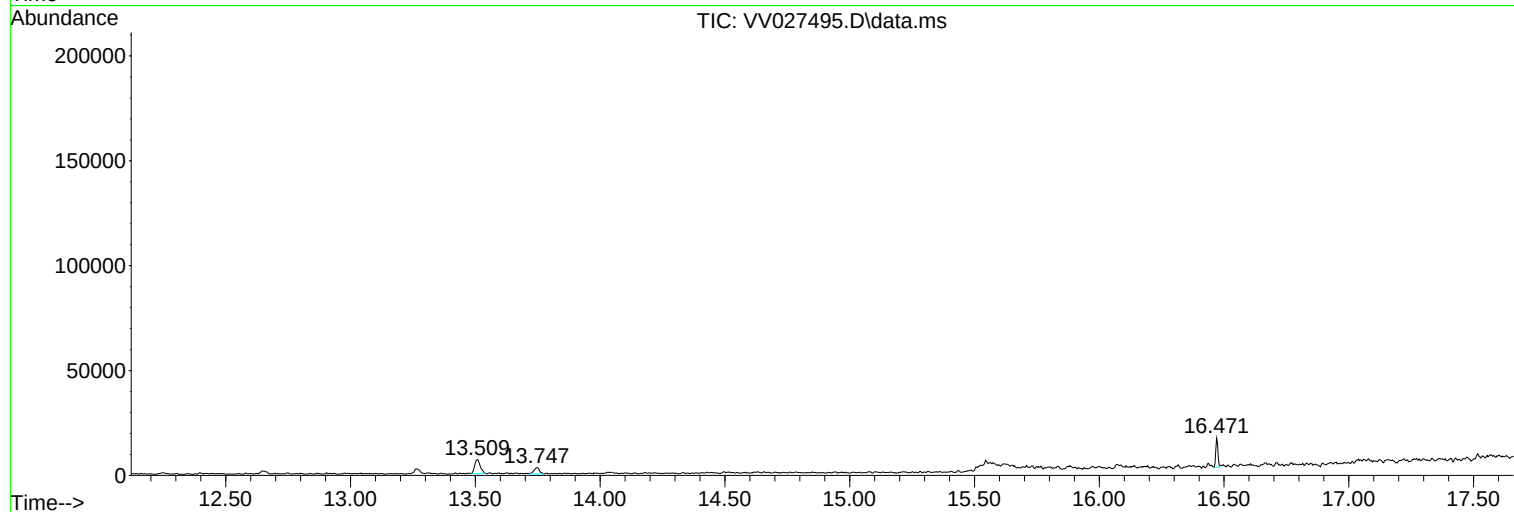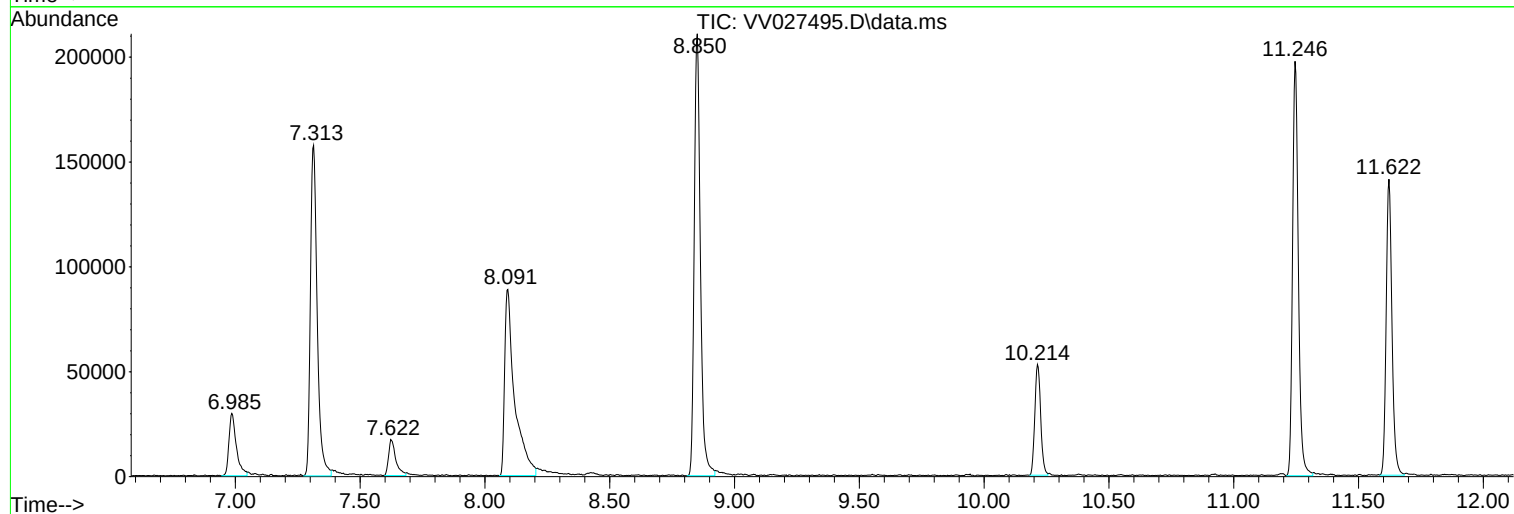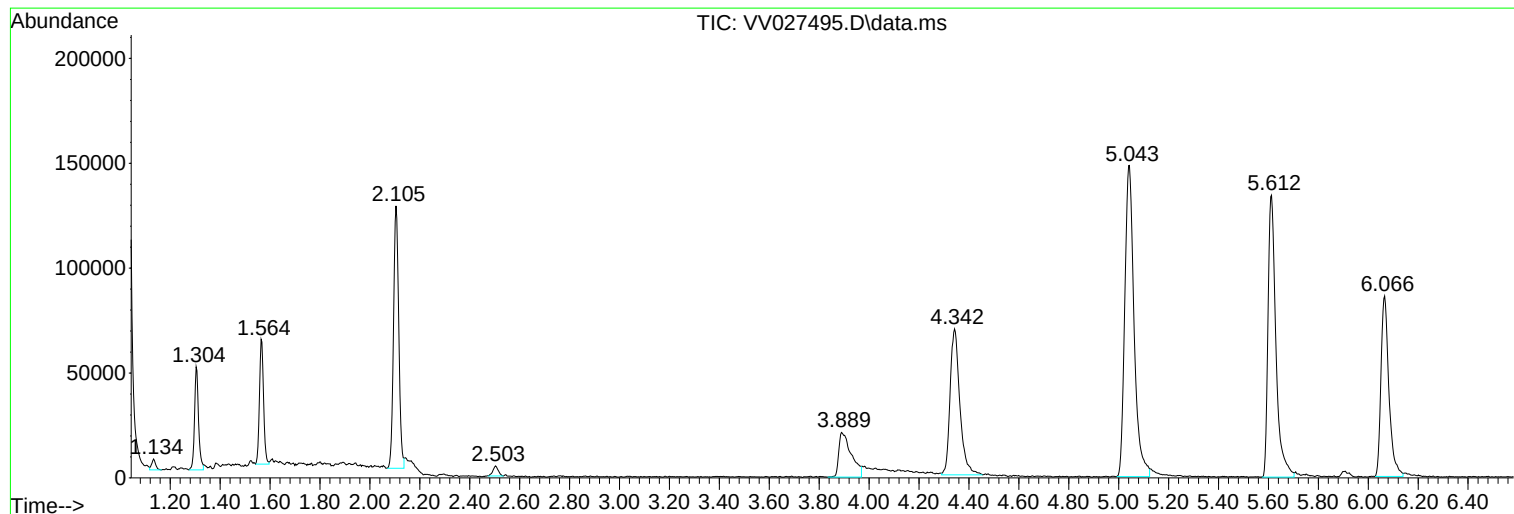

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027495.D
Acq On : 25 Aug 2022 09:49
Operator : SY/MD
Sample : VV0825WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027495.D
Acq On : 25 Aug 2022 09:49
Operator : SY/MD
Sample : VV0825WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
