

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027500.D
 Acq On : 25 Aug 2022 17:24
 Operator : SY/MD
 Sample : N4370-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E83

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	11	15	32	rVB	8979	15569	4.27%	0.537%
2	1.304	71	82	97	rBV	54520	64763	17.75%	2.234%
3	1.417	113	117	123	rVB3	4309	4160	1.14%	0.143%
4	1.564	157	163	175	rVB	49796	57800	15.84%	1.994%
5	2.105	321	331	345	rVB	115886	169423	46.44%	5.843%
6	3.896	880	888	908	rBV2	20122	65130	17.85%	2.246%
7	4.349	1010	1029	1047	rBV	66563	168597	46.21%	5.815%
8	5.047	1231	1246	1290	rBV2	135951	364821	100.00%	12.583%
9	5.616	1411	1423	1458	rBV	115486	257477	70.58%	8.880%
10	6.069	1551	1564	1594	rBV2	80502	181690	49.80%	6.267%
11	6.989	1840	1850	1873	rBV2	32148	66936	18.35%	2.309%
12	7.317	1941	1952	1973	rBV	145863	271872	74.52%	9.377%
13	7.629	2039	2049	2064	rBV3	18017	35471	9.72%	1.223%
14	7.937	2136	2145	2147	rBV3	4273	5455	1.50%	0.188%
15	8.091	2184	2193	2227	rBV	104181	256705	70.36%	8.854%
16	8.854	2415	2430	2451	rBV	185151	315792	86.56%	10.892%
17	10.217	2843	2854	2867	rBV	53895	86934	23.83%	2.998%
18	10.384	2895	2906	2917	rVB3	8711	14913	4.09%	0.514%
19	11.249	3163	3175	3196	rBV	174826	278814	76.42%	9.616%
20	11.625	3281	3292	3313	rBV	132177	217047	59.49%	7.486%




Sum of corrected areas: 2899369

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027500.D
Acq On : 25 Aug 2022 17:24
Operator : SY/MD
Sample : N4370-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

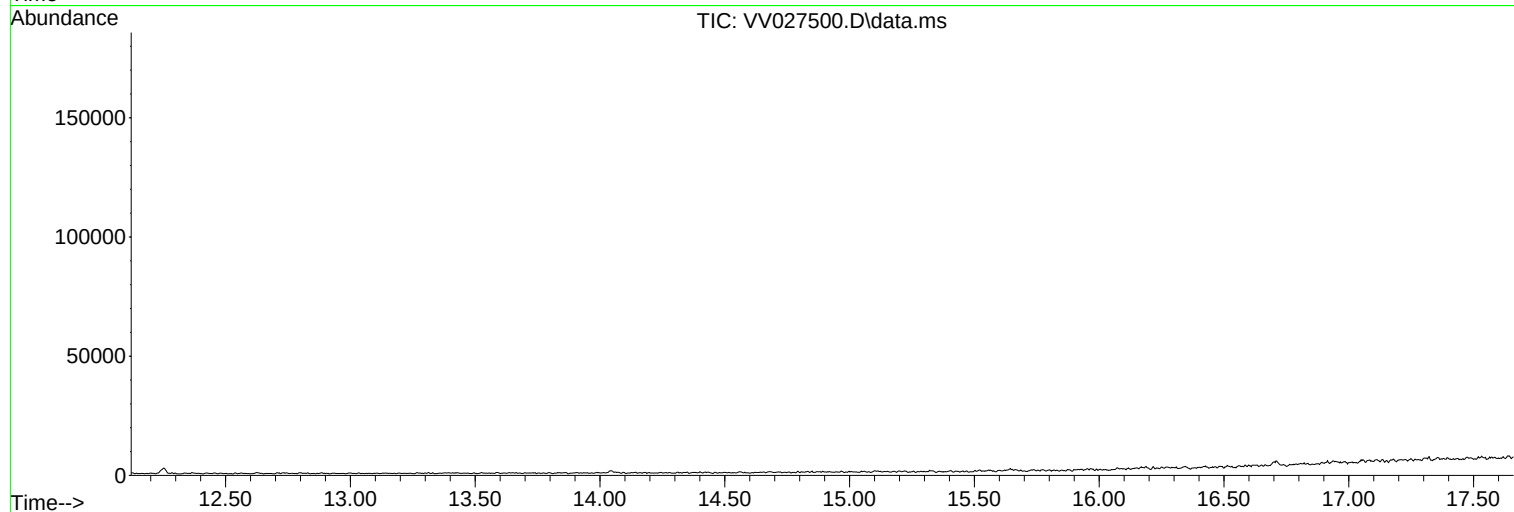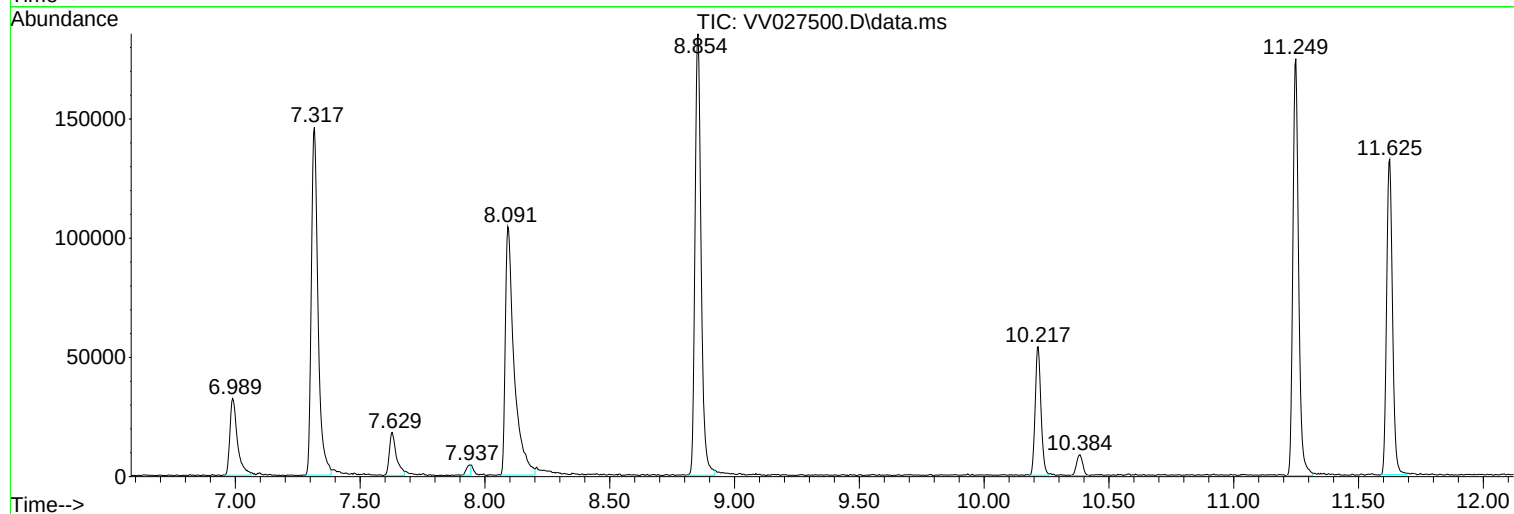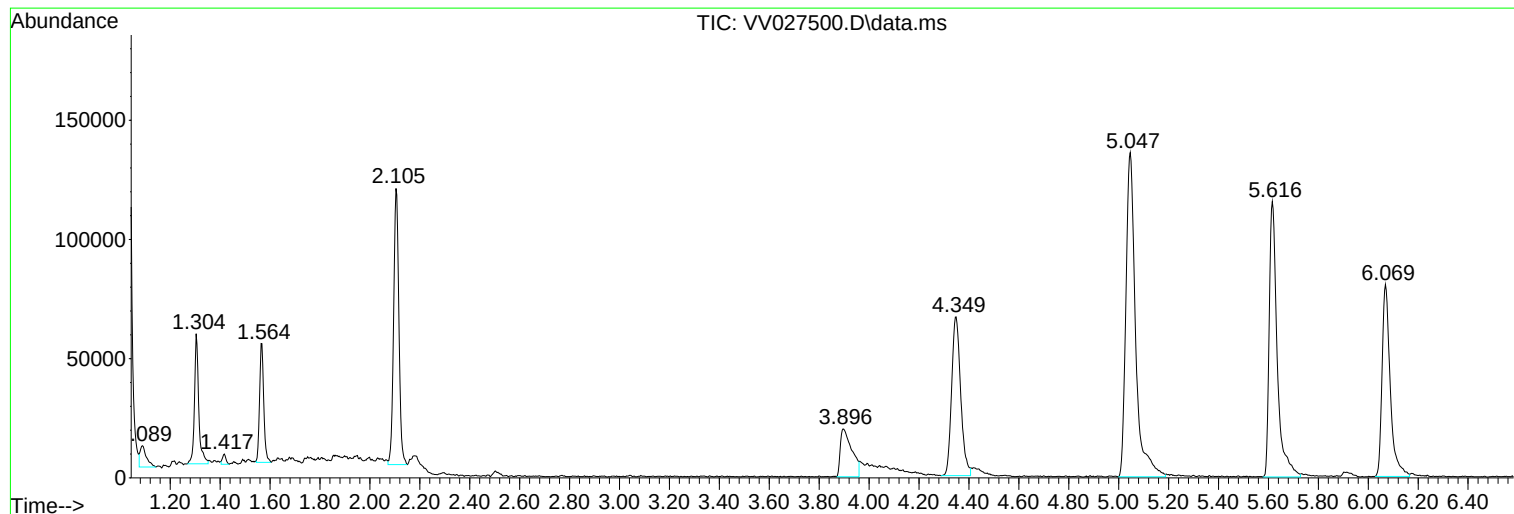

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027500.D
Acq On : 25 Aug 2022 17:24
Operator : SY/MD
Sample : N4370-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027500.D
Acq On : 25 Aug 2022 17:24
Operator : SY/MD
Sample : N4370-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc