

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027511.D
 Acq On : 25 Aug 2022 22:20
 Operator : SY/MD
 Sample : N4367-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E93

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	95	rBV	51609	60302	10.46%	1.586%
2	1.564	156	163	173	rBV	47284	52582	9.12%	1.383%
3	2.105	321	331	345	rBV	102041	153301	26.59%	4.033%
4	2.169	348	351	369	rVB	7491	15897	2.76%	0.418%
5	2.761	526	535	546	rBV5	9473	18426	3.20%	0.485%
6	3.905	880	891	914	rBV3	37706	126270	21.90%	3.322%
7	4.349	1012	1029	1049	rBV2	63337	165716	28.75%	4.360%
8	5.047	1230	1246	1280	rBV2	131016	345194	59.88%	9.081%
9	5.616	1412	1423	1454	rBV	130850	286692	49.73%	7.542%
10	5.912	1502	1515	1544	rBV	274908	576444	100.00%	15.165%
11	6.069	1551	1564	1593	rBV2	79317	175052	30.37%	4.605%
12	6.989	1840	1850	1870	rBV2	30219	62302	10.81%	1.639%
13	7.317	1935	1952	1972	rBV	140209	259904	45.09%	6.838%
14	7.629	2039	2049	2062	rBV3	16571	32491	5.64%	0.855%
15	7.976	2137	2157	2177	rBV2	133589	242762	42.11%	6.387%
16	8.092	2182	2193	2227	rBV	108159	255058	44.25%	6.710%
17	8.850	2419	2429	2449	rBV	209598	354681	61.53%	9.331%
18	10.217	2843	2854	2869	rBV	53534	85570	14.84%	2.251%
19	10.384	2895	2906	2918	rVB4	13556	21635	3.75%	0.569%
20	11.249	3162	3175	3197	rBV	192884	305813	53.05%	8.045%
21	11.622	3280	3291	3308	rBV	127206	204990	35.56%	5.393%




Sum of corrected areas: 3801082

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027511.D
Acq On : 25 Aug 2022 22:20
Operator : SY/MD
Sample : N4367-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

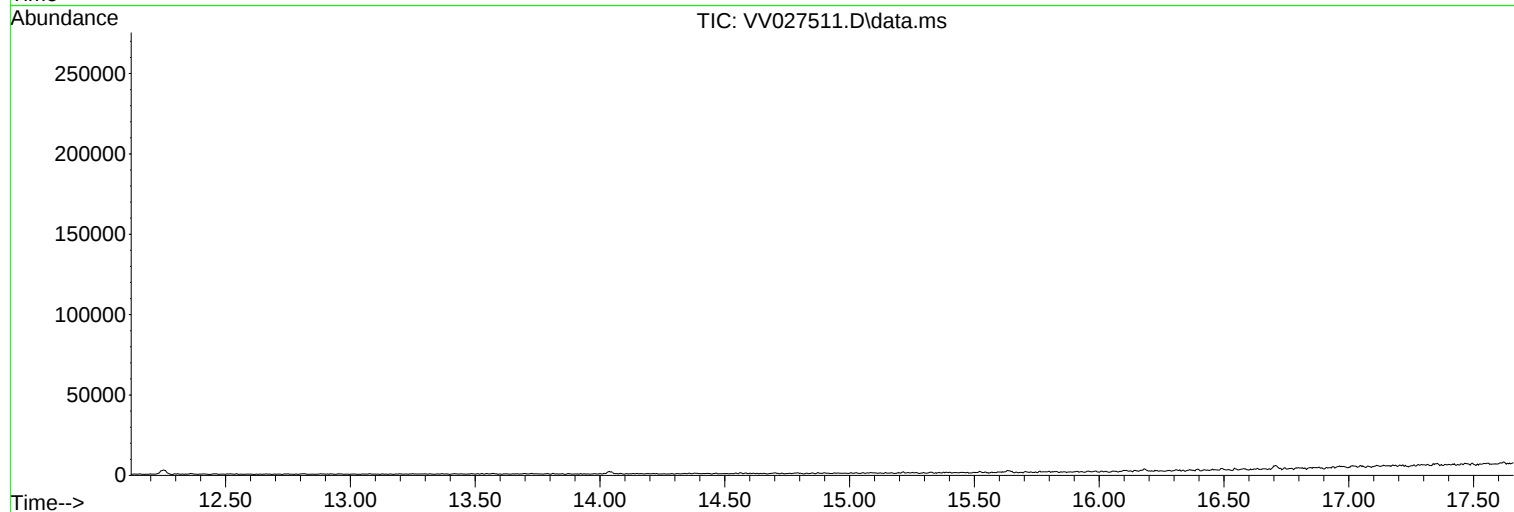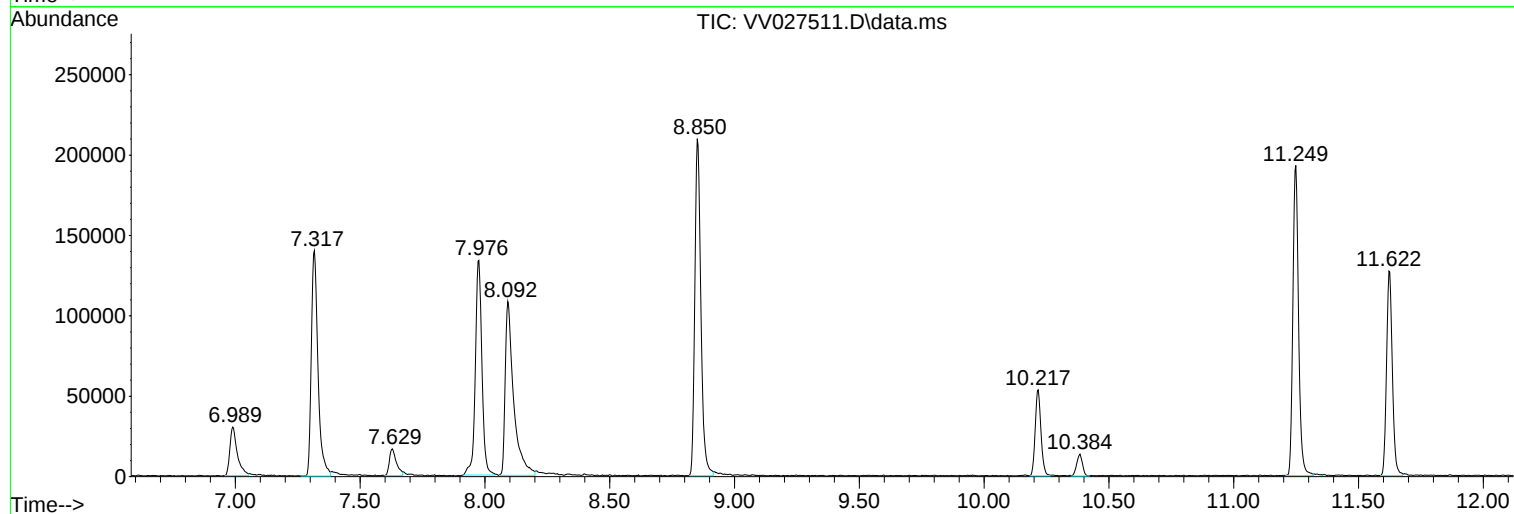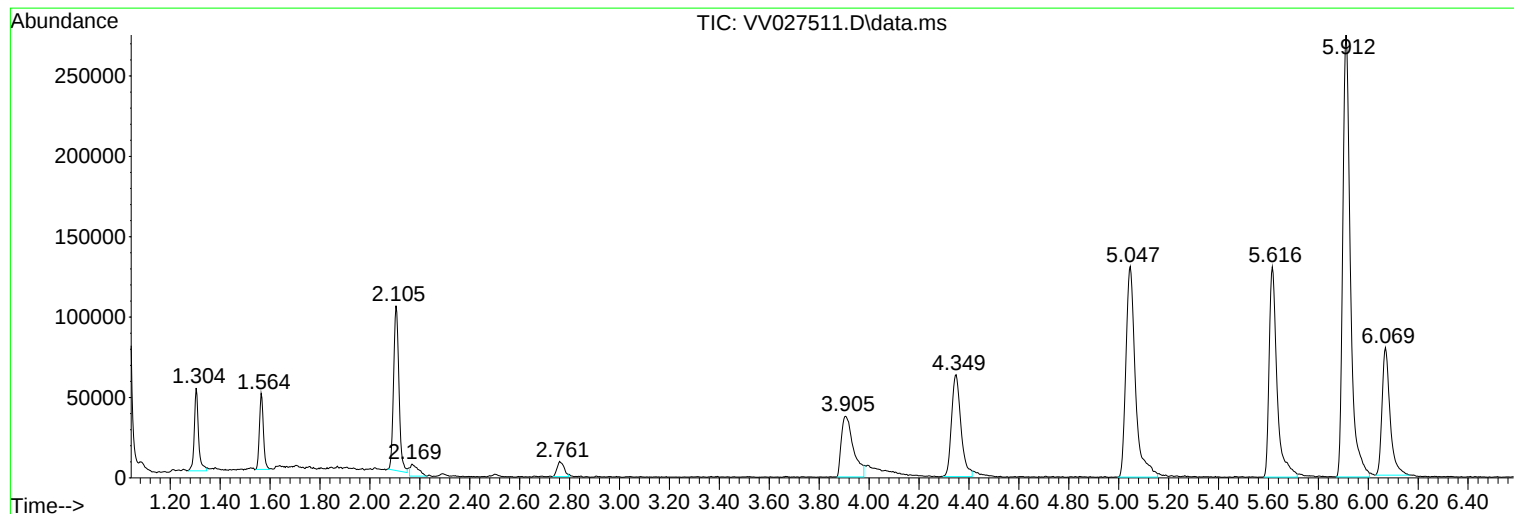

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027511.D
Acq On : 25 Aug 2022 22:20
Operator : SY/MD
Sample : N4367-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027511.D
Acq On : 25 Aug 2022 22:20
Operator : SY/MD
Sample : N4367-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc