

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027512.D
 Acq On : 25 Aug 2022 22:45
 Operator : SY/MD
 Sample : N4367-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E94

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rBV	43689	53460	9.18%	1.414%
2	1.564	157	163	176	rVB	48205	58458	10.04%	1.547%
3	2.105	319	331	343	rVB	112503	161373	27.72%	4.270%
4	2.764	526	536	549	rBV6	8986	18022	3.10%	0.477%
5	3.908	879	892	907	rBV4	35844	105247	18.08%	2.785%
6	4.346	1013	1028	1046	rBV2	64811	166441	28.59%	4.404%
7	5.047	1230	1246	1278	rBV2	130213	348161	59.81%	9.212%
8	5.616	1412	1423	1461	rBV	131817	294633	50.62%	7.796%
9	5.911	1502	1515	1549	rBV	279818	582100	100.00%	15.402%
10	6.069	1551	1564	1591	rVV	80409	174381	29.96%	4.614%
11	6.989	1840	1850	1877	rBV2	30610	64382	11.06%	1.703%
12	7.317	1941	1952	1975	rBV	141073	262842	45.15%	6.955%
13	7.628	2039	2049	2066	rBV	17092	34165	5.87%	0.904%
14	7.972	2135	2156	2177	rBV	129275	236588	40.64%	6.260%
15	8.095	2182	2194	2236	rBV	95534	251827	43.26%	6.663%
16	8.850	2419	2429	2454	rBV	209792	359373	61.74%	9.509%
17	10.217	2843	2854	2870	rBV	51933	84958	14.60%	2.248%
18	10.381	2895	2905	2915	rBV4	7481	11573	1.99%	0.306%
19	11.249	3164	3175	3198	rBV	191798	306975	52.74%	8.122%
20	11.625	3281	3292	3311	rBV	124752	204490	35.13%	5.411%




Sum of corrected areas: 3779449

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027512.D
Acq On : 25 Aug 2022 22:45
Operator : SY/MD
Sample : N4367-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

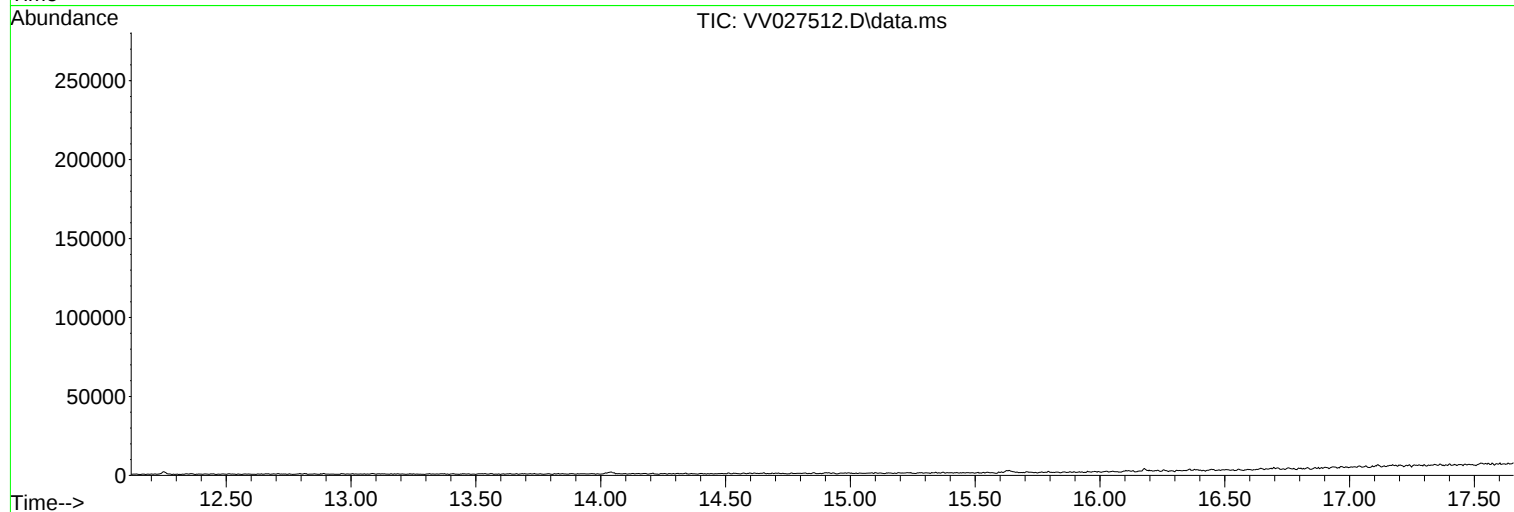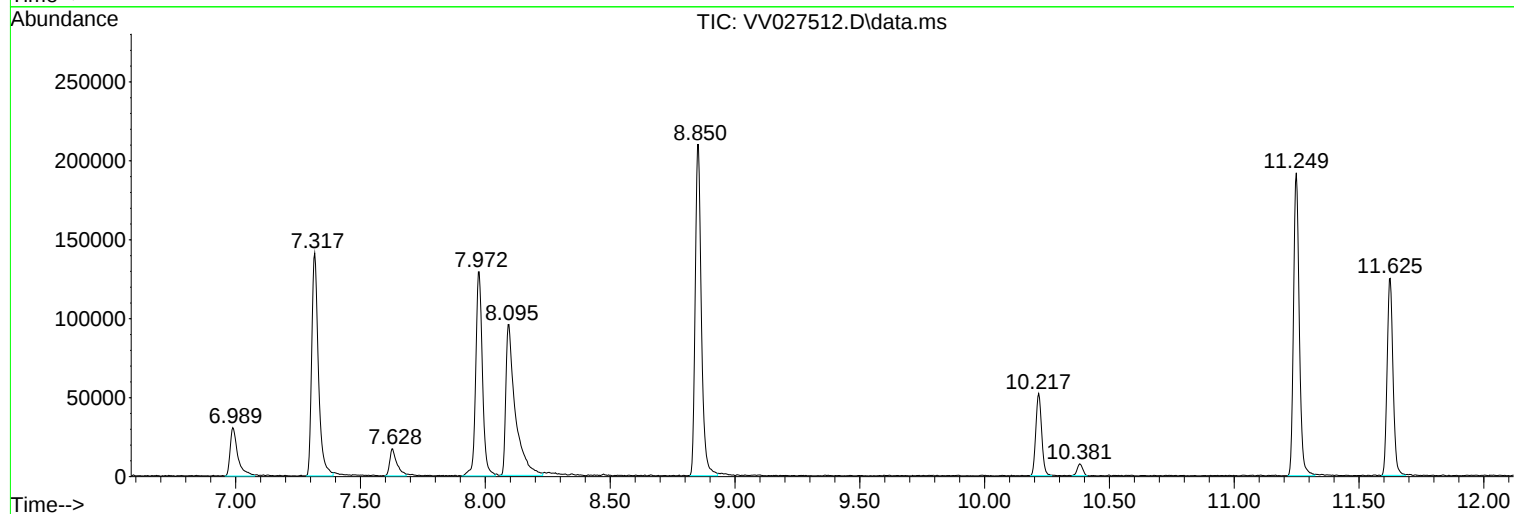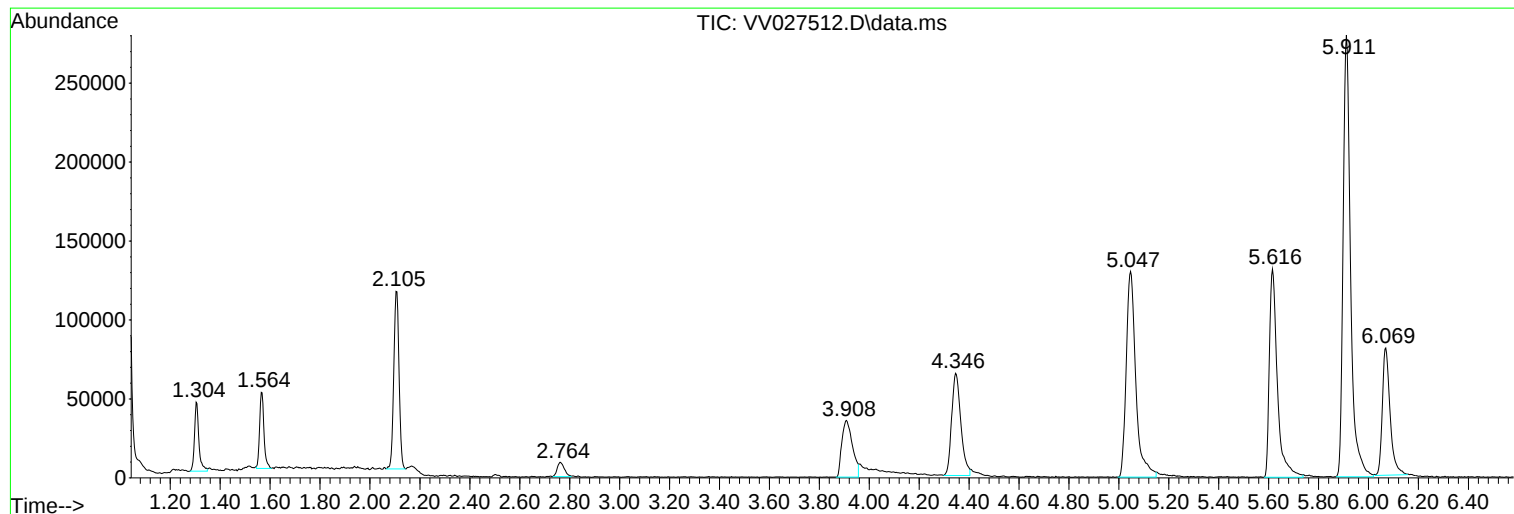

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027512.D
Acq On : 25 Aug 2022 22:45
Operator : SY/MD
Sample : N4367-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027512.D
Acq On : 25 Aug 2022 22:45
Operator : SY/MD
Sample : N4367-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc