

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027517.D
 Acq On : 26 Aug 2022 00:48
 Operator : SY/MD
 Sample : N4367-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rBV	43459	52039	5.01%	1.218%
2	1.519	130	149	153	rBV2	19441	55471	5.34%	1.299%
3	1.564	158	163	177	rVB	55370	73780	7.10%	1.727%
4	2.105	322	331	342	rVB	118854	173633	16.70%	4.065%
5	3.905	878	891	917	rBV5	48988	162437	15.63%	3.803%
6	4.346	1013	1028	1054	rBV	70415	188671	18.15%	4.418%
7	5.043	1228	1245	1287	rBV2	139105	367610	35.37%	8.607%
8	5.616	1411	1423	1454	rBV	137033	302450	29.10%	7.082%
9	5.918	1507	1517	1539	rBV3	18379	41482	3.99%	0.971%
10	6.069	1551	1564	1588	rBV	81452	180136	17.33%	4.218%
11	6.992	1841	1851	1866	rBV	25153	50740	4.88%	1.188%
12	7.317	1940	1952	1972	rBV	145719	274726	26.43%	6.432%
13	7.628	2041	2049	2070	rBV2	13245	26699	2.57%	0.625%
14	7.972	2134	2156	2183	rBV	601779	1039457	100.00%	24.338%
15	8.091	2183	2193	2226	rVV	126633	264817	25.48%	6.200%
16	8.850	2417	2429	2453	rBV	222764	376832	36.25%	8.823%
17	10.217	2842	2854	2875	rBV2	53343	90020	8.66%	2.108%
18	10.381	2894	2905	2915	rVB3	6447	10598	1.02%	0.248%
19	11.249	3163	3175	3195	rBV	202465	323223	31.10%	7.568%
20	11.622	3280	3291	3310	rBV	136036	216166	20.80%	5.061%




Sum of corrected areas: 4270987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027517.D
Acq On : 26 Aug 2022 00:48
Operator : SY/MD
Sample : N4367-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

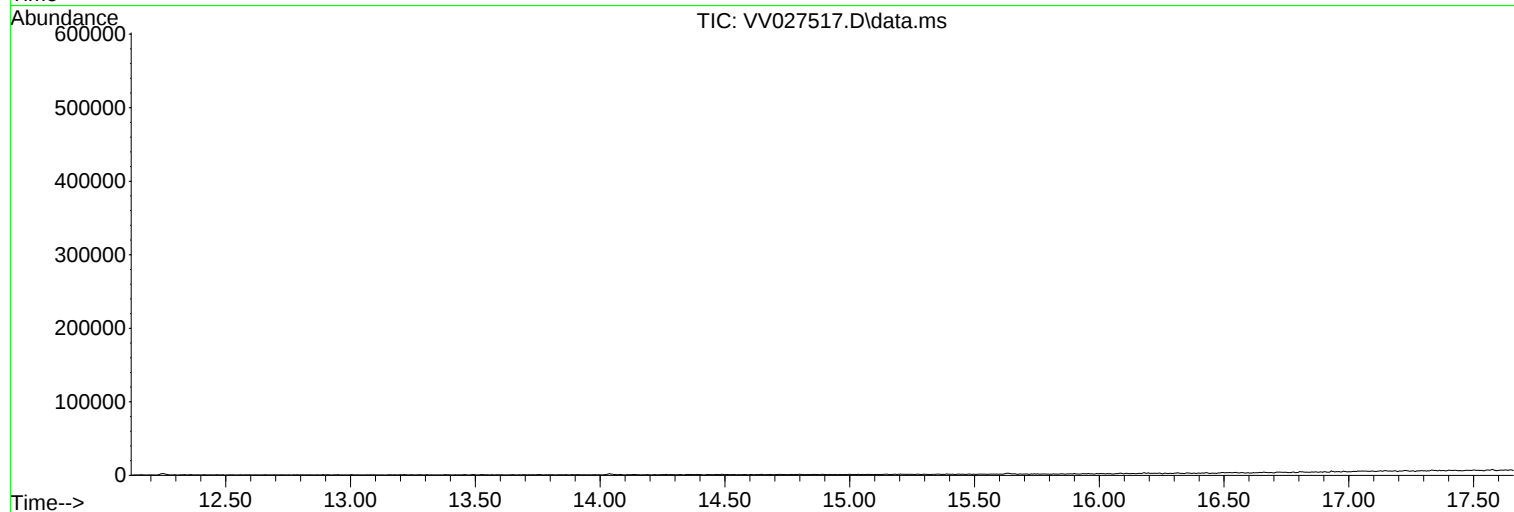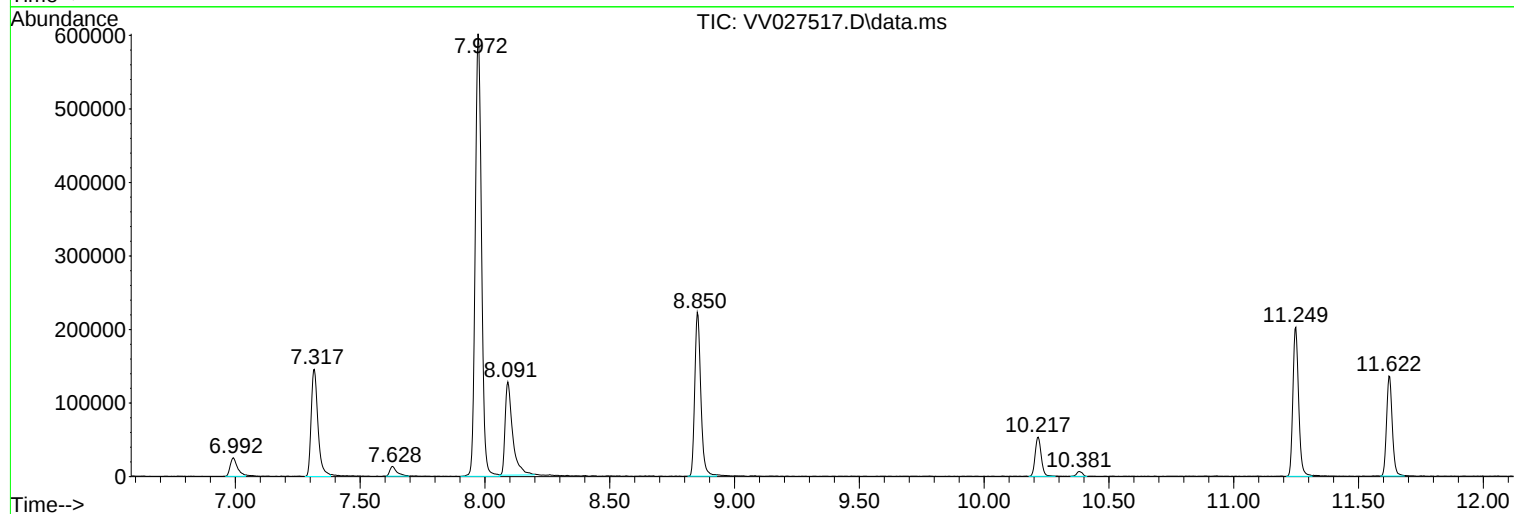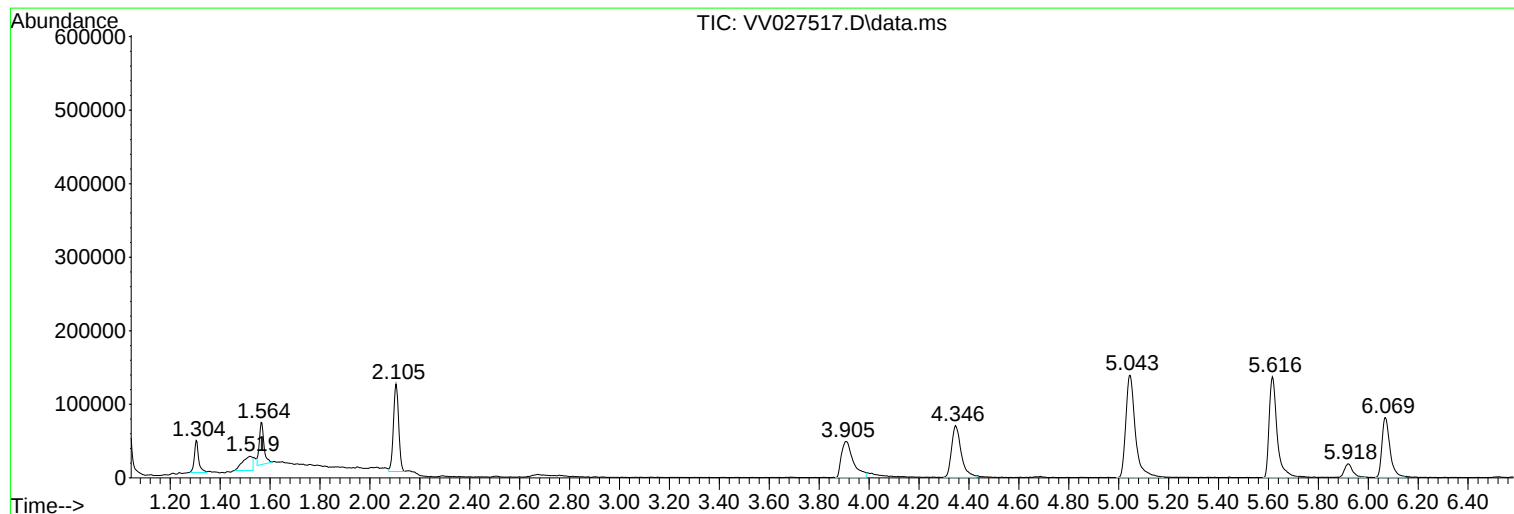

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027517.D
Acq On : 26 Aug 2022 00:48
Operator : SY/MD
Sample : N4367-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027517.D
Acq On : 26 Aug 2022 00:48
Operator : SY/MD
Sample : N4367-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc