

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027518.D
 Acq On : 26 Aug 2022 01:12
 Operator : SY/MD
 Sample : N4367-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rVB	47493	51225	7.78%	1.371%
2	1.516	127	148	153	rBV2	16362	50965	7.74%	1.364%
3	1.564	158	163	173	rVB	52282	63368	9.63%	1.696%
4	2.105	323	331	343	rVB	117362	168980	25.67%	4.523%
5	3.895	879	888	925	rBV2	25769	98674	14.99%	2.641%
6	4.346	1011	1028	1061	rBV2	67568	178353	27.10%	4.774%
7	5.047	1228	1246	1276	rBV3	135038	356590	54.17%	9.545%
8	5.616	1412	1423	1451	rBV2	142210	307700	46.75%	8.236%
9	6.069	1547	1564	1586	rBV	83408	182843	27.78%	4.894%
10	6.989	1837	1850	1873	rBV3	25014	54054	8.21%	1.447%
11	7.317	1941	1952	1972	rBV	148316	272145	41.34%	7.285%
12	7.628	2039	2049	2070	rBV3	13813	27150	4.12%	0.727%
13	7.972	2135	2156	2180	rBV	381037	658242	100.00%	17.620%
14	8.091	2184	2193	2219	rBV	121426	253261	38.48%	6.779%
15	8.850	2419	2429	2445	rBV	220498	369986	56.21%	9.904%
16	10.217	2843	2854	2867	rBV	54849	87258	13.26%	2.336%
17	10.381	2896	2905	2916	rBV3	8414	12977	1.97%	0.347%
18	11.249	3162	3175	3192	rBV	207882	324186	49.25%	8.678%
19	11.622	3278	3291	3312	rBV	135470	217856	33.10%	5.832%




Sum of corrected areas: 3735813

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027518.D
Acq On : 26 Aug 2022 01:12
Operator : SY/MD
Sample : N4367-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

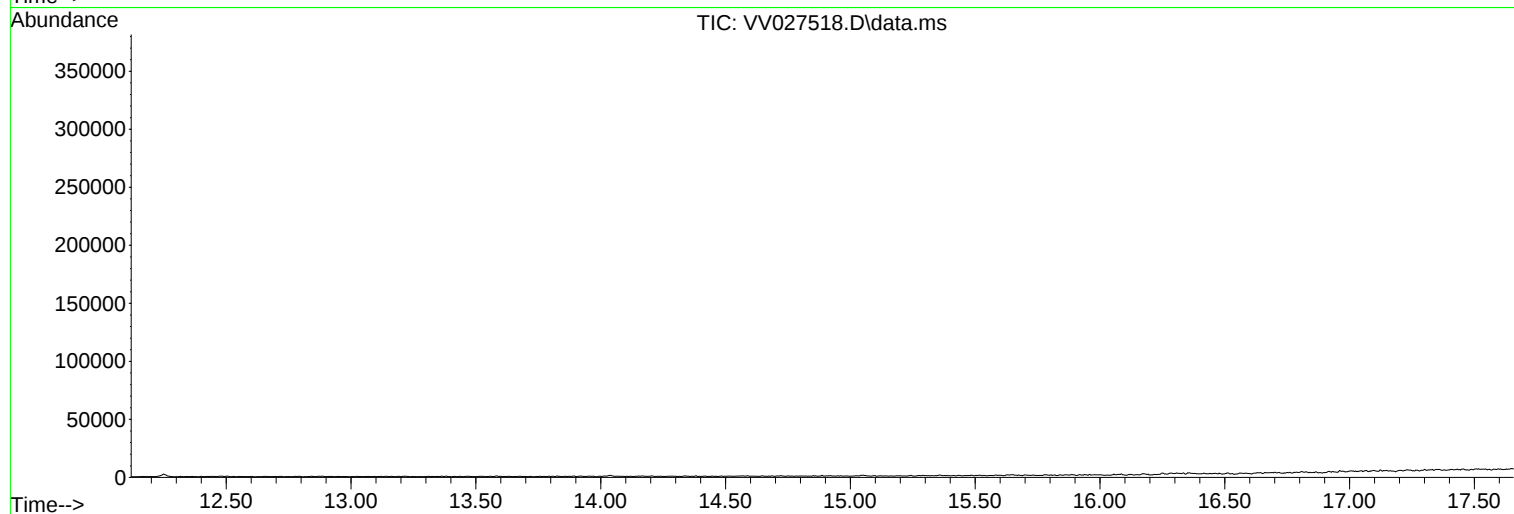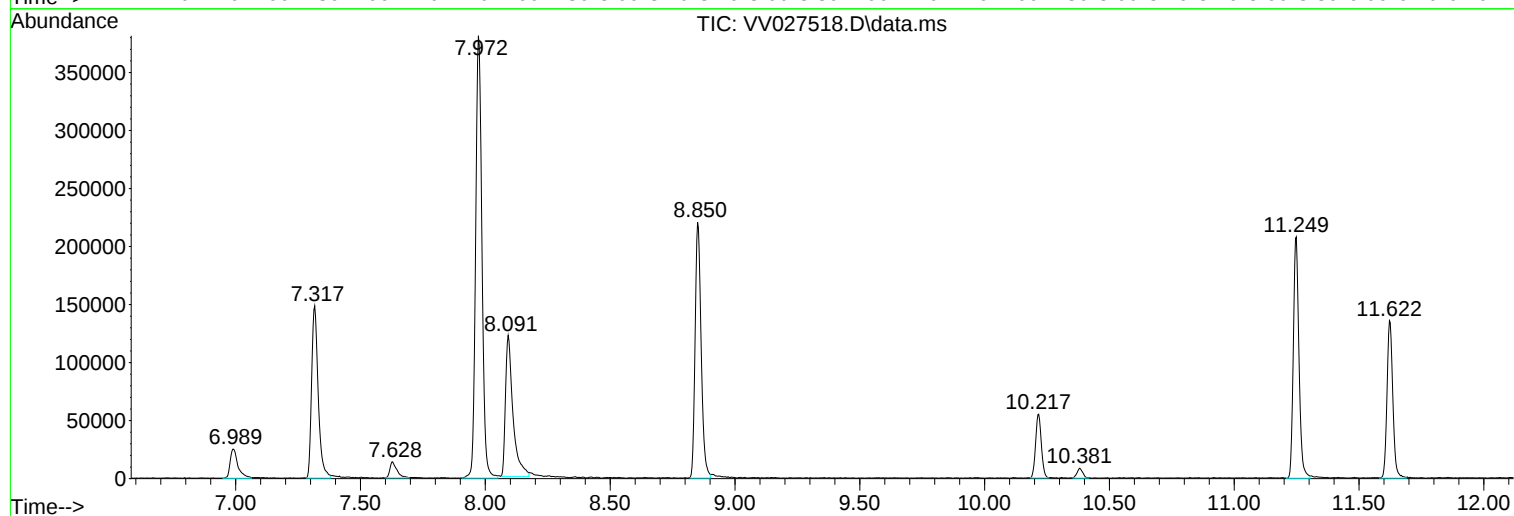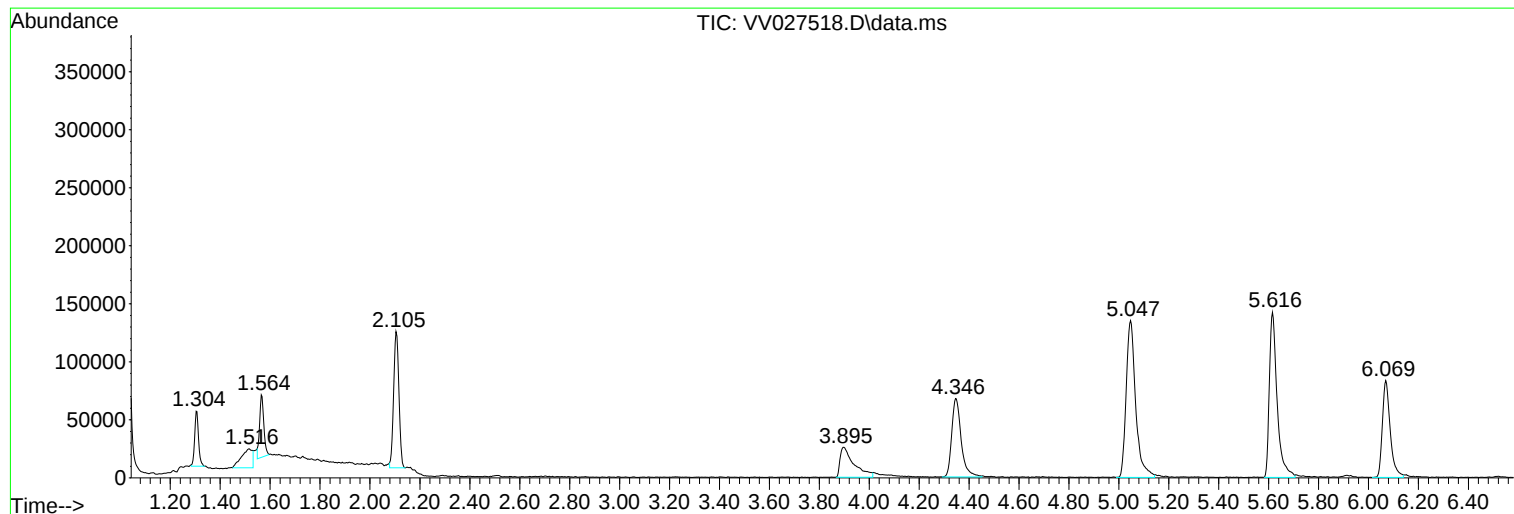

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027518.D
Acq On : 26 Aug 2022 01:12
Operator : SY/MD
Sample : N4367-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027518.D
Acq On : 26 Aug 2022 01:12
Operator : SY/MD
Sample : N4367-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc