

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027521.D
 Acq On : 26 Aug 2022 02:26
 Operator : SY/MD
 Sample : N4370-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E90

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	103	rBV	42972	56438	4.54%	1.314%
2	1.564	157	163	175	rBV	52335	58142	4.68%	1.353%
3	2.105	322	331	346	rVB	118633	171906	13.84%	4.001%
4	2.767	521	537	572	rBV	570799	1242403	100.00%	28.917%
5	3.896	879	888	914	rBV	19484	68880	5.54%	1.603%
6	4.346	1011	1028	1057	rBV	69017	177359	14.28%	4.128%
7	5.047	1230	1246	1275	rBV4	136427	357186	28.75%	8.314%
8	5.291	1306	1322	1336	rBV5	5641	13900	1.12%	0.324%
9	5.616	1411	1423	1458	rBV	144373	314752	25.33%	7.326%
10	6.066	1552	1563	1588	rBV	82347	178400	14.36%	4.152%
11	6.989	1841	1850	1876	rBV2	27327	56641	4.56%	1.318%
12	7.317	1941	1952	1975	rBV	145296	274958	22.13%	6.400%
13	7.629	2039	2049	2070	rBV2	14620	30137	2.43%	0.701%
14	8.092	2183	2193	2228	rBV	102872	259170	20.86%	6.032%
15	8.850	2418	2429	2455	rBV	222346	382505	30.79%	8.903%
16	10.217	2841	2854	2868	rBV2	54553	89838	7.23%	2.091%
17	10.384	2896	2906	2920	rVB2	9302	14941	1.20%	0.348%
18	11.249	3163	3175	3191	rBV	205923	329796	26.55%	7.676%
19	11.622	3281	3291	3313	rBV	133903	219071	17.63%	5.099%




Sum of corrected areas: 4296423

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027521.D
Acq On : 26 Aug 2022 02:26
Operator : SY/MD
Sample : N4370-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

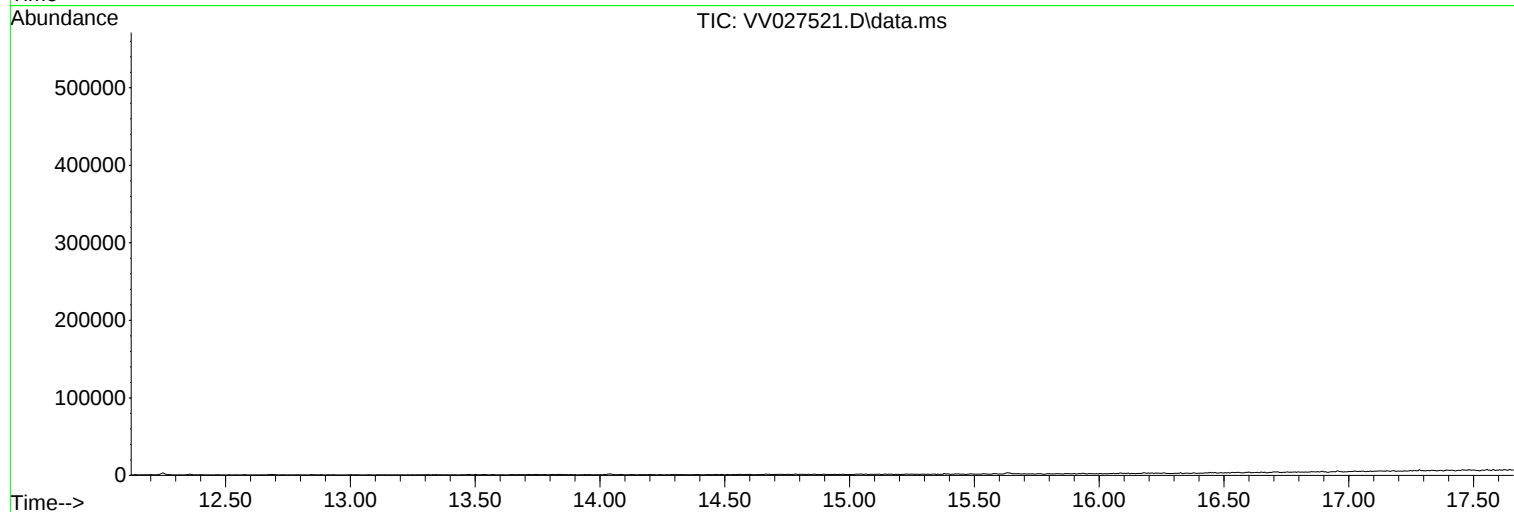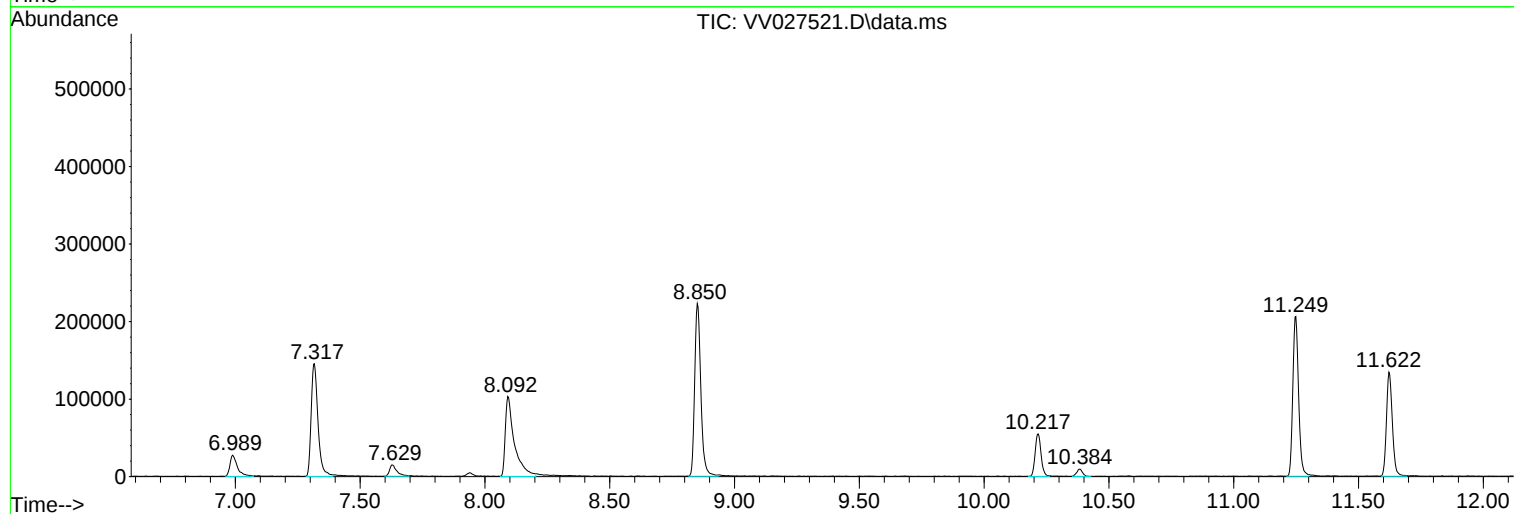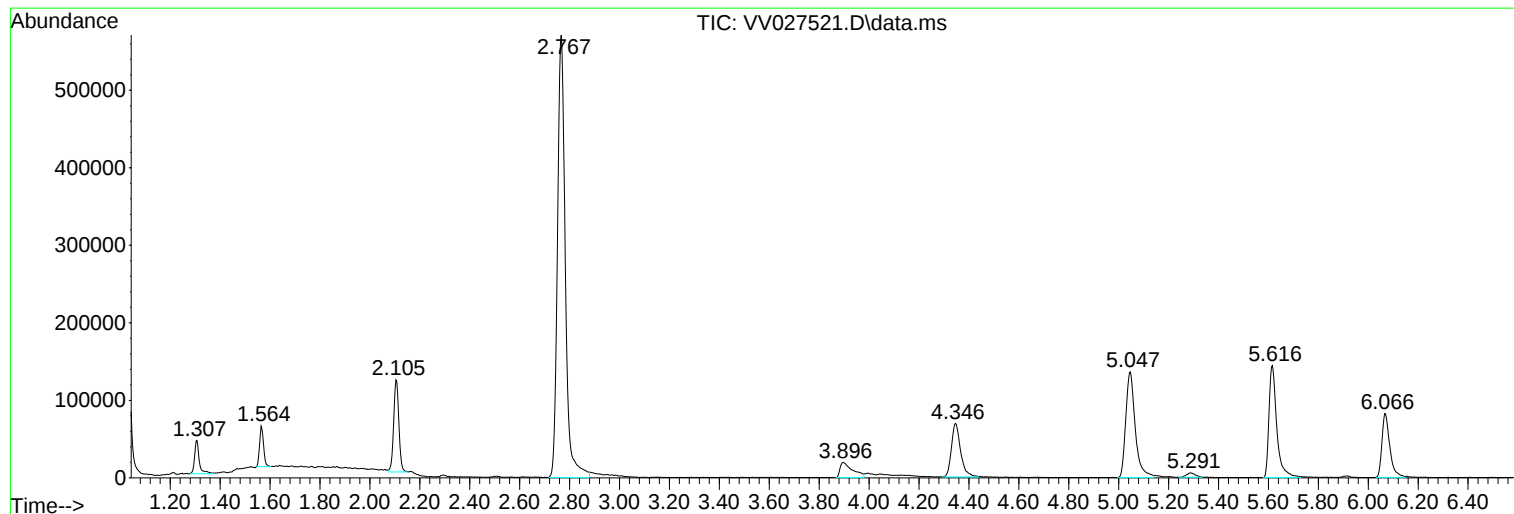

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027521.D
Acq On : 26 Aug 2022 02:26
Operator : SY/MD
Sample : N4370-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027521.D
Acq On : 26 Aug 2022 02:26
Operator : SY/MD
Sample : N4370-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E90

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc