

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
 Data File : VV027523.D
 Acq On : 26 Aug 2022 03:15
 Operator : SY/MD
 Sample : N4370-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F11

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	93	rBV	45592	54108	14.07%	1.774%
2	1.568	156	164	173	rBV	54713	64805	16.85%	2.125%
3	2.108	322	332	342	rVB	114875	161892	42.09%	5.308%
4	2.503	444	455	464	rBV6	2380	4556	1.18%	0.149%
5	3.896	880	888	919	rBV	18952	70195	18.25%	2.302%
6	4.346	1013	1028	1064	rBV2	71728	192480	50.04%	6.311%
7	5.047	1230	1246	1273	rBV2	138909	357772	93.01%	11.730%
8	5.616	1411	1423	1445	rBV	138280	301007	78.25%	9.869%
9	6.069	1551	1564	1597	rBV2	83234	182934	47.56%	5.998%
10	6.989	1840	1850	1865	rBV3	28032	55094	14.32%	1.806%
11	7.317	1940	1952	1971	rBV	148417	271508	70.58%	8.902%
12	7.632	2039	2050	2065	rBV2	15165	31476	8.18%	1.032%
13	7.937	2135	2145	2147	rBV3	4295	5773	1.50%	0.189%
14	8.092	2184	2193	2226	rBV	101314	258129	67.10%	8.463%
15	8.850	2417	2429	2459	rBV	225331	384670	100.00%	12.612%
16	10.214	2843	2853	2875	rBV	53978	87998	22.88%	2.885%
17	10.381	2895	2905	2919	rVB3	8724	14015	3.64%	0.460%
18	11.246	3164	3174	3199	rBV	208031	333985	86.82%	10.951%
19	11.622	3280	3291	3307	rBV	132561	217540	56.55%	7.133%




Sum of corrected areas: 3049937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027523.D
Acq On : 26 Aug 2022 03:15
Operator : SY/MD
Sample : N4370-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

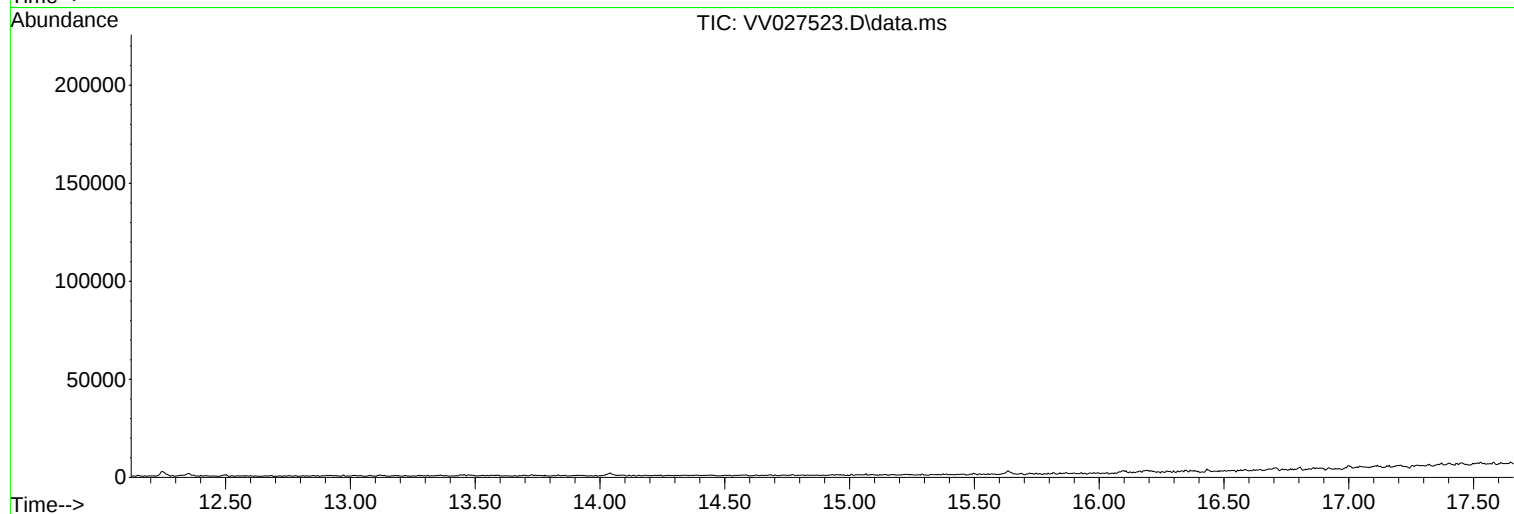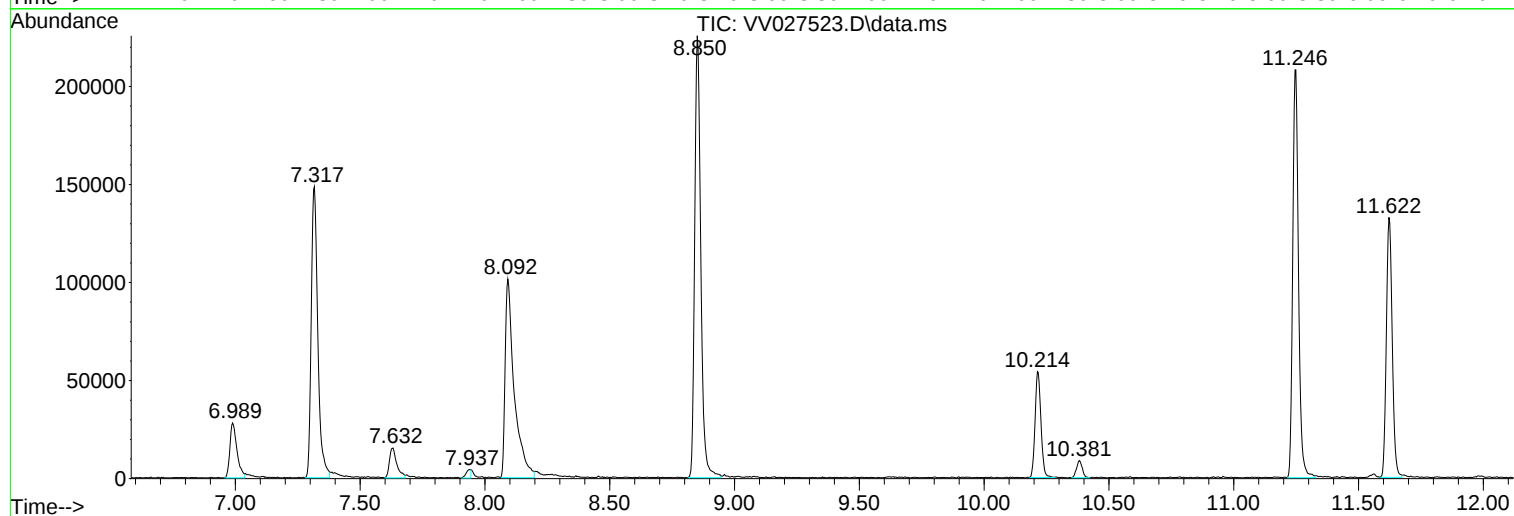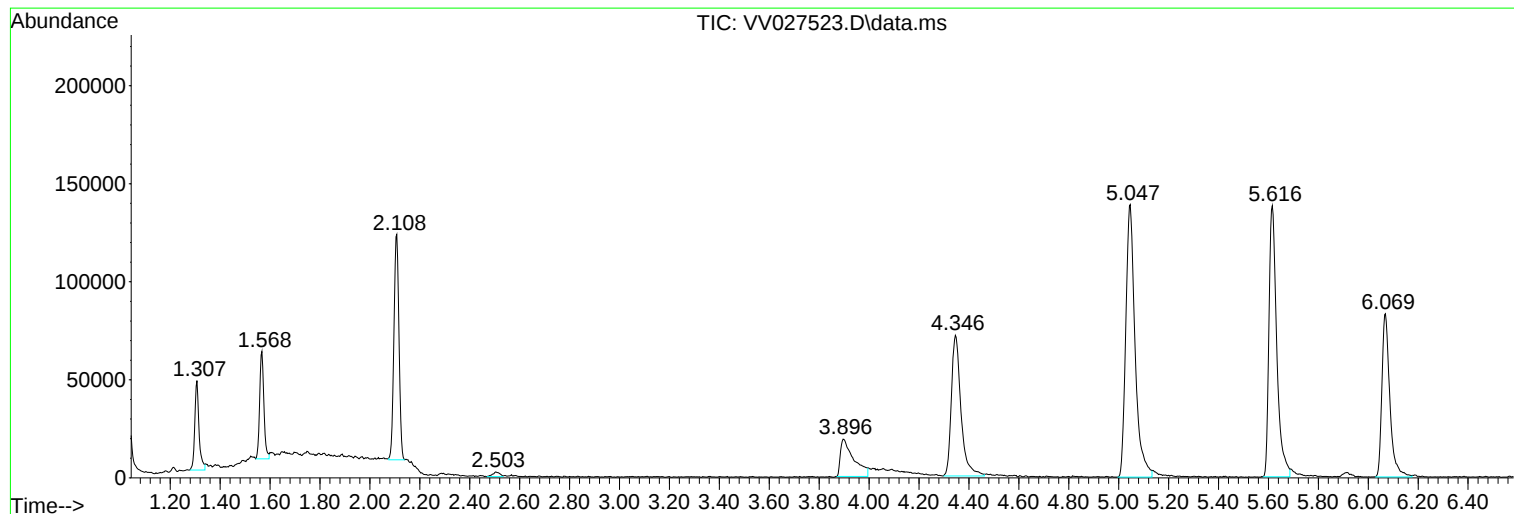

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027523.D
Acq On : 26 Aug 2022 03:15
Operator : SY/MD
Sample : N4370-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082522\
Data File : VV027523.D
Acq On : 26 Aug 2022 03:15
Operator : SY/MD
Sample : N4370-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc