

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031926.D
 Acq On : 25 Aug 2023 11:00
 Operator : SY/MD
 Sample : 04108-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 26 00:51:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	226638	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	221622	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	117030	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	56580	39.891	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.780%
7) Chloroethane-d5	1.532	69	53219	42.802	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.063	65	27399	41.254	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.500%
21) 2-Butanone-d5	3.799	46	122707	109.997	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.000%
24) Chloroform-d	4.256	84	139153	44.885	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.780%
26) 1,2-Dichloroethane-d4	4.947	65	96675	46.989	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.980%
32) Benzene-d6	4.963	84	283220	46.833	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.660%
36) 1,2-Dichloropropane-d6	5.992	67	97254	49.964	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.920%
41) Toluene-d8	7.246	98	254376	45.652	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.300%
43) trans-1,3-Dichloroprop...	7.558	79	47272	46.857	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.720%
47) 2-Hexanone-d5	8.030	63	62621	104.966	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.970%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	131932	52.452	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.900%
66) 1,2-Dichlorobenzene-d4	11.564	152	101811	47.723	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.440%
Target Compounds						
61) 1,2,3-Trichloropropane	11.188	75	16073	7.269	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031926.D
Acq On : 25 Aug 2023 11:00
Operator : SY/MD
Sample : 04108-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 26 00:51:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

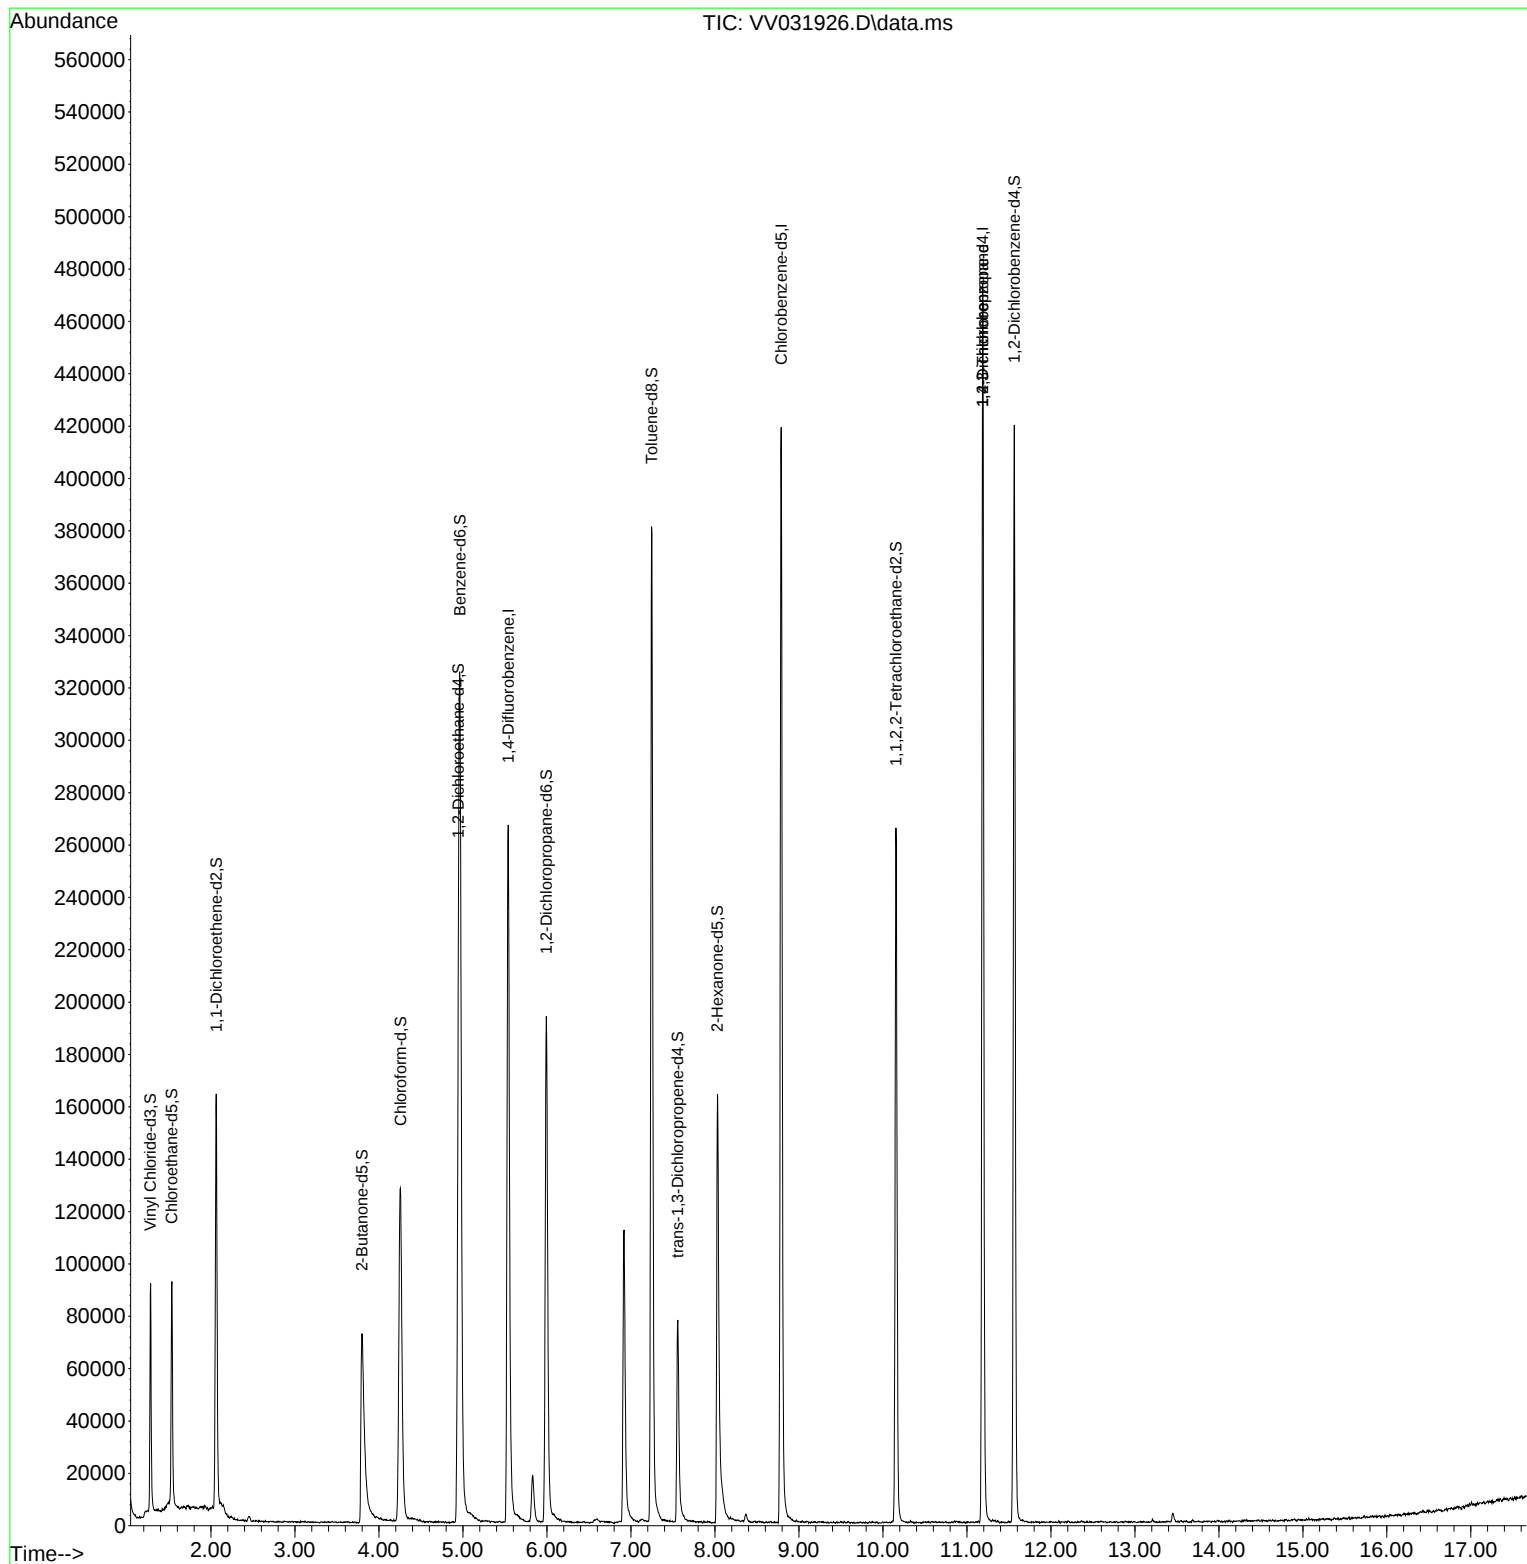

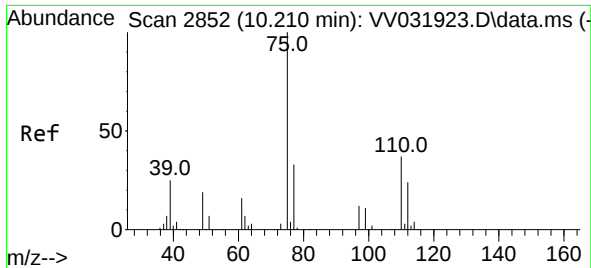

#61
 1,2,3-Trichloropropane
 Concen: 7.269 ug/L
 RT: 11.188 min Scan# 3156
 Delta R.T. 0.978 min
 Lab File: VV031926.D
 Acq: 25 Aug 2023 11:00

Instrument :
 MSVOA_V
 ClientSampleId :

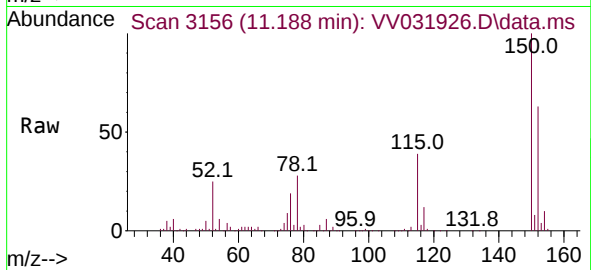

Tgt Ion	Ratio	Lower	Upper
75	100		
77	33.8	25.7	38.5
110	2.5	30.3	45.5

