

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW082523\
 Data File : VW031928.D
 Acq On : 25 Aug 2023 12:04
 Operator : SY/MD
 Sample : 04113-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 26 00:51:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	237369	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	229744	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	121049	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	60968	41.041	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.080%		
7) Chloroethane-d5	1.532	69	59850	45.959	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.920%		
11) 1,1-Dichloroethene-d2	2.063	65	30060	43.214	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.420%		
21) 2-Butanone-d5	3.796	46	123571	105.763	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	105.760%		
24) Chloroform-d	4.252	84	148180	45.636	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.280%		
26) 1,2-Dichloroethane-d4	4.947	65	101731	47.211	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.420%		
32) Benzene-d6	4.963	84	306886	48.953	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.900%		
36) 1,2-Dichloropropane-d6	5.992	67	102691	50.893	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.780%		
41) Toluene-d8	7.246	98	271190	46.949	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.900%		
43) trans-1,3-Dichloroprop...	7.558	79	48688	46.554	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.100%		
47) 2-Hexanone-d5	8.030	63	60748	98.227	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.230%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	129420	49.634	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.260%		
66) 1,2-Dichlorobenzene-d4	11.564	152	106780	48.390	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.780%		
Target Compounds					Qvalue	
13) Acetone	2.127	43	8619	8.288	ug/L	96
44) trans-1,3-Dichloropropene	7.558	75	2193	0.750	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031928.D
Acq On : 25 Aug 2023 12:04
Operator : SY/MD
Sample : 04113-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 26 00:51:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

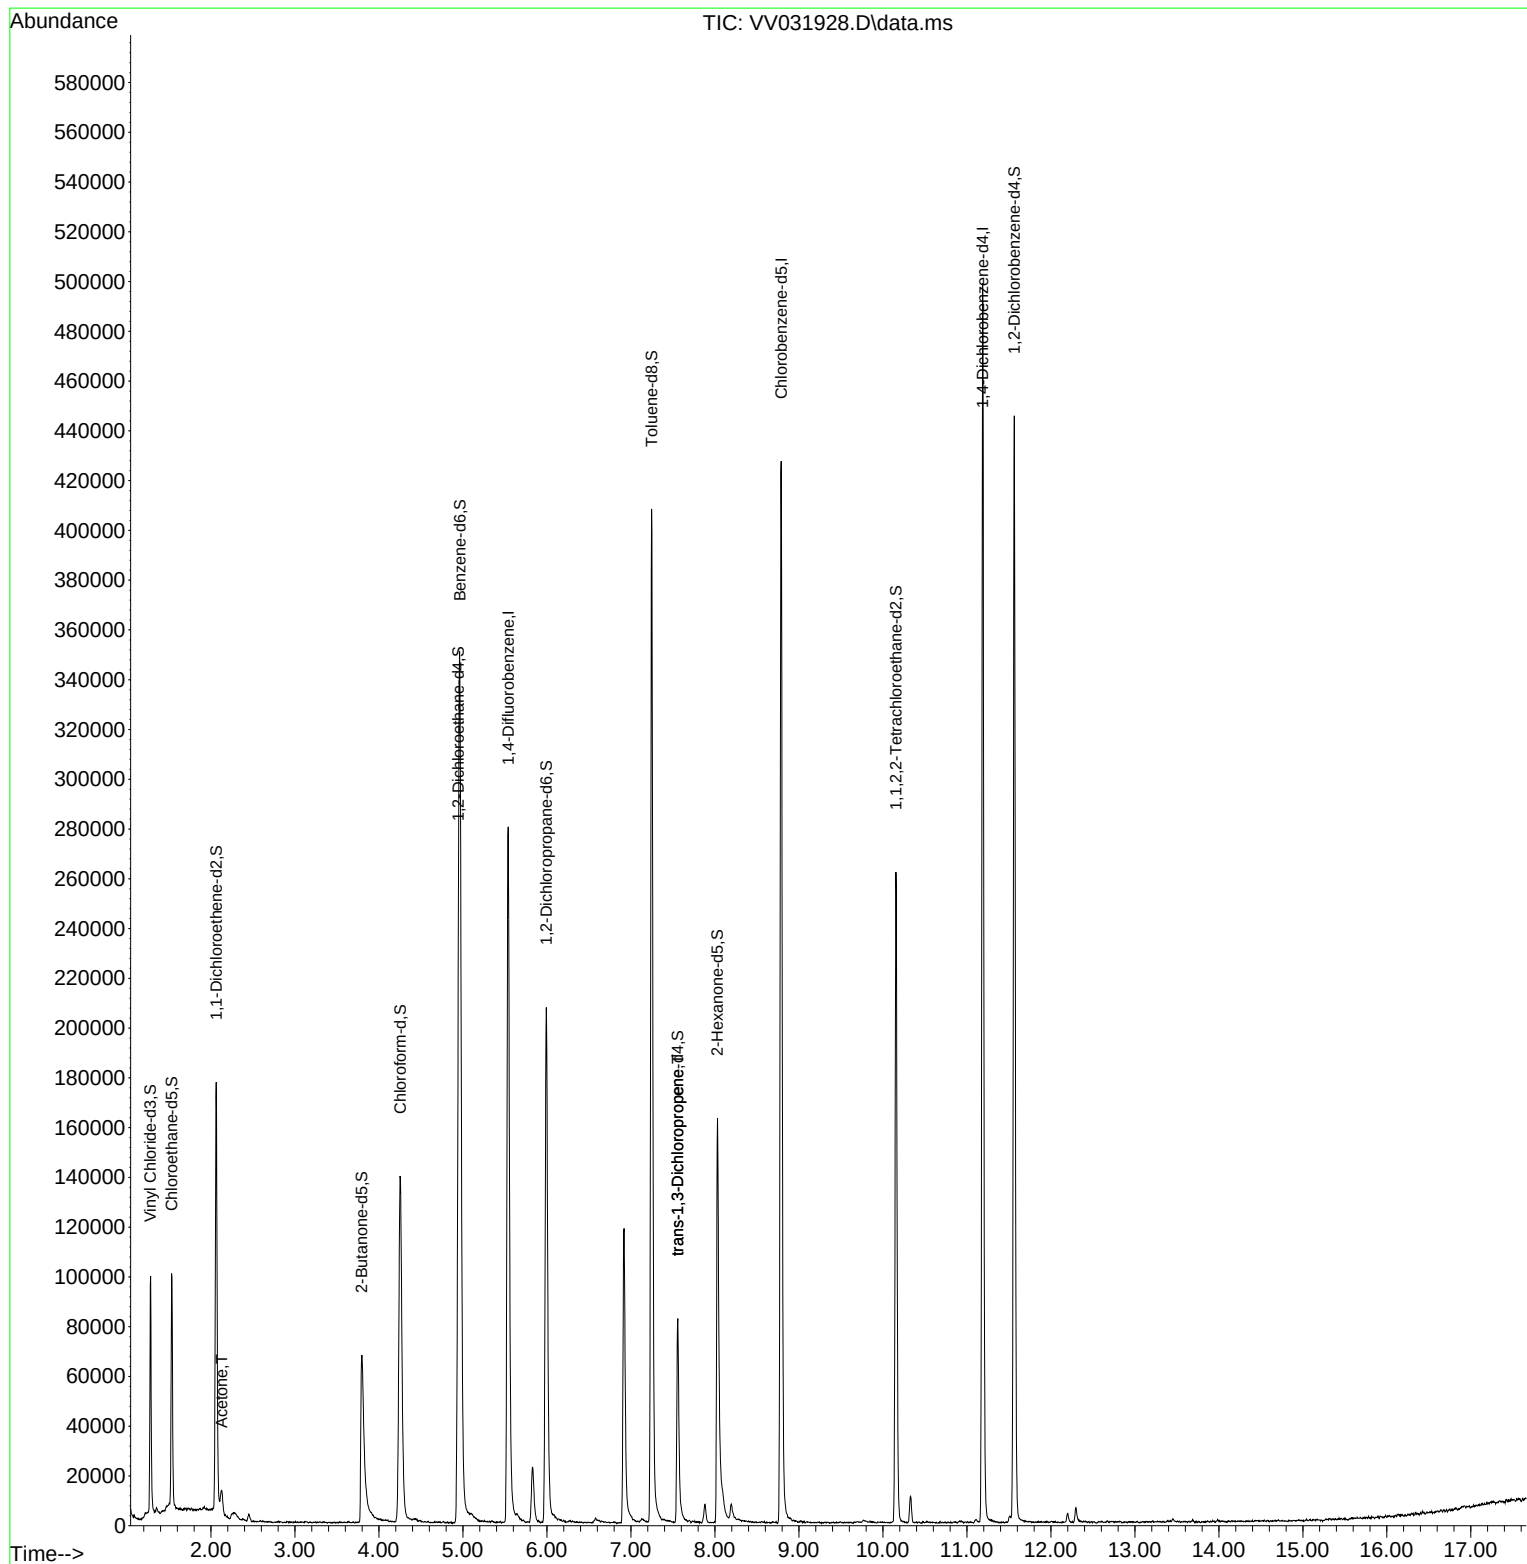

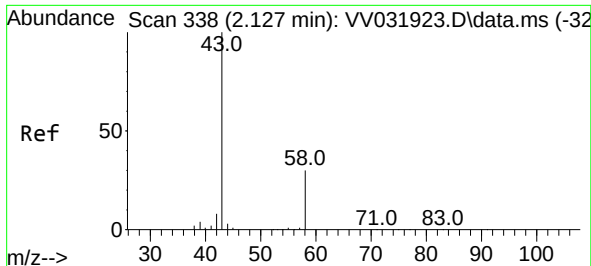

#13

Acetone

Concen: 8.288 ug/L

RT: 2.127 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV031928.D

Acq: 25 Aug 2023 12:04

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 8619

Ion Ratio Lower Upper

43 100

58 32.5 0.0 61.0

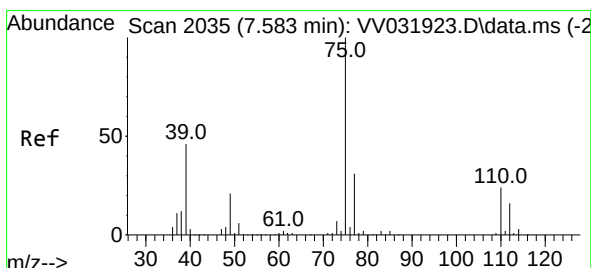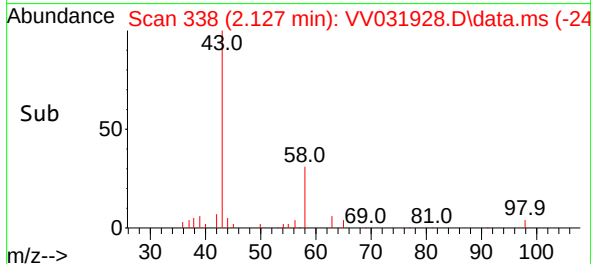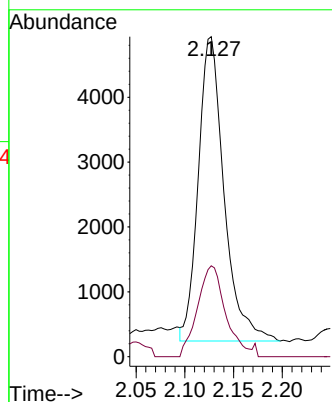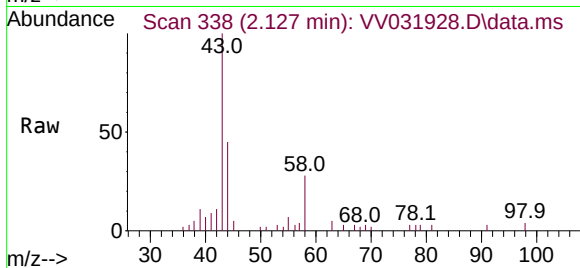

#44

trans-1,3-Dichloropropene

Concen: 0.750 ug/L

RT: 7.558 min Scan# 2027

Delta R.T. -0.026 min

Lab File: VV031928.D

Acq: 25 Aug 2023 12:04

Tgt Ion: 75 Resp: 2193

Ion Ratio Lower Upper

75 100

77 41.2 22.5 41.9

