




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031930.D
 Acq On : 25 Aug 2023 12:51
 Operator : SY/MD
 Sample : 04138-01ME
 Misc : 5.54g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 26 00:52:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/28/2023
 Supervised By :Semsettin Yesilyurt 08/28/2023

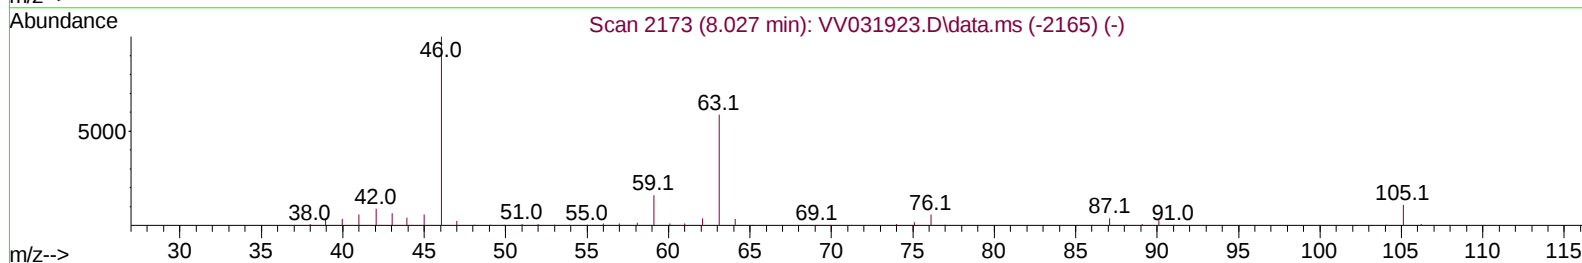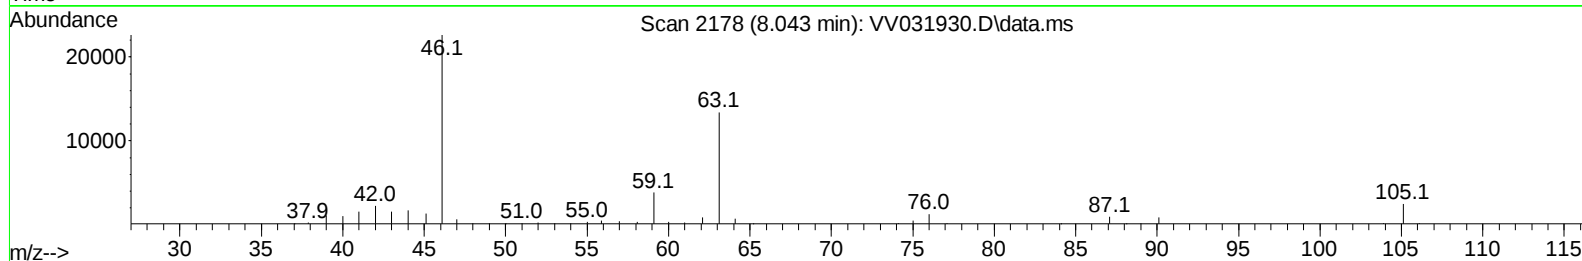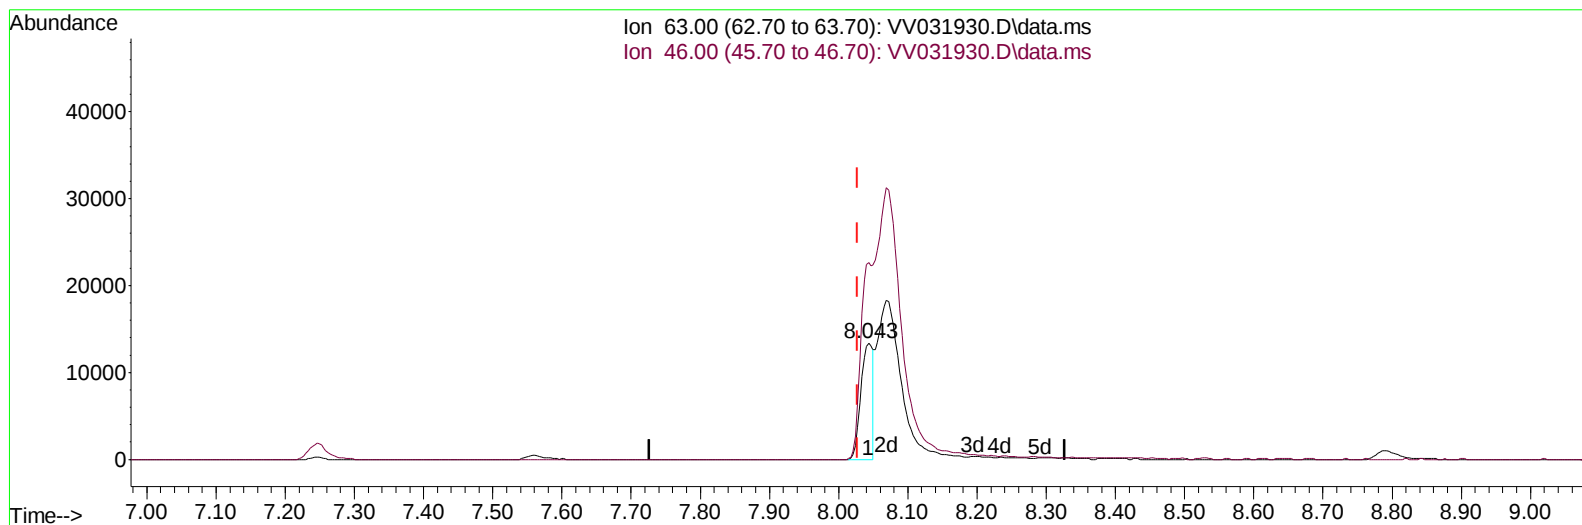

TIC: VV031930.D\data.ms

(47) 2-Hexanone-d5 (S)

8.043min (+ 0.016) 23.44 ug/L

response 16584

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	147.21
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031930.D
 Acq On : 25 Aug 2023 12:51
 Operator : SY/MD
 Sample : 04138-01ME
 Misc : 5.54g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHQ5ME

Manual IntegrationsAPPROVED

Quant Time: Aug 26 00:52:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 08/28/2023
 Supervised By :Semsettin Yesilyurt 08/28/2023

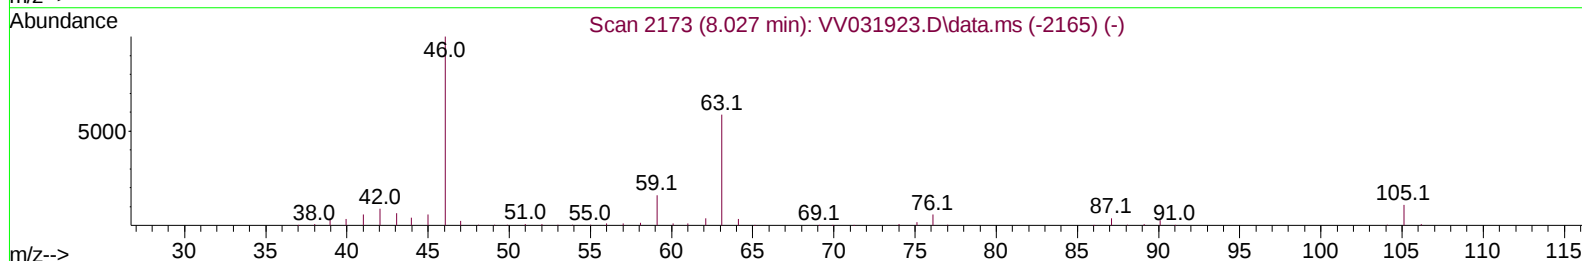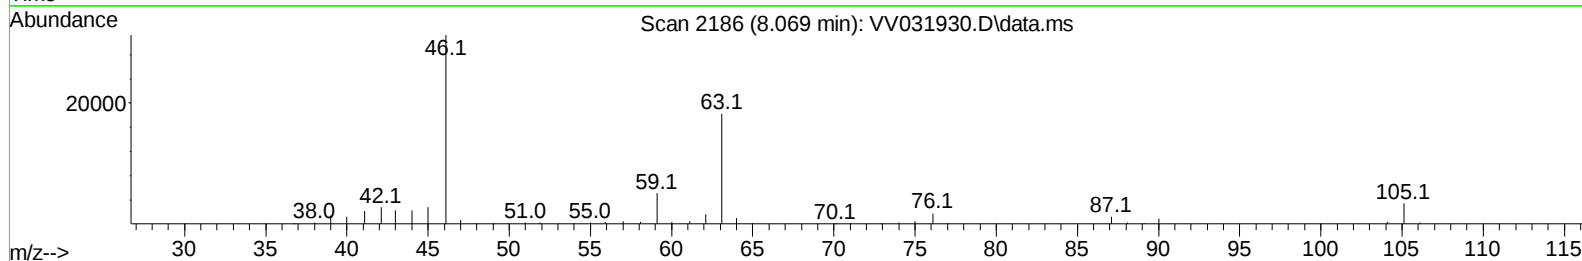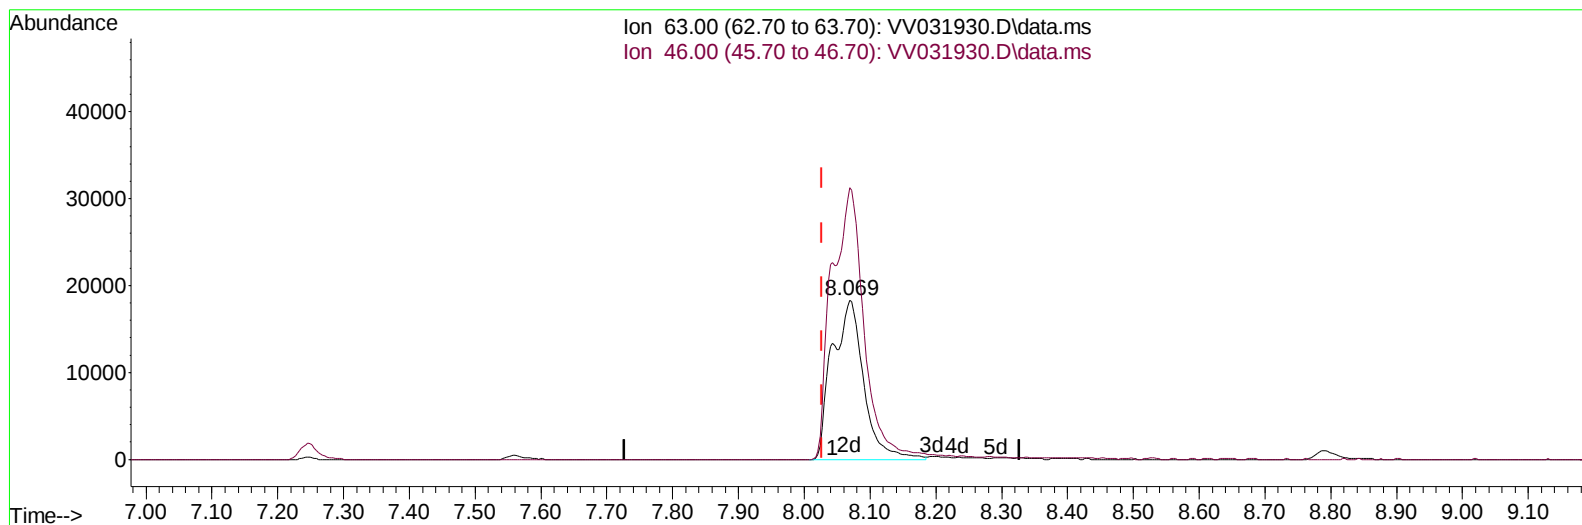

TIC: VV031930.D\data.ms

(47) 2-Hexanone-d5 (S)

8.069min (+ 0.042) 86.28 ug/L m

response 61042

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	39.99#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031930.D
 Acq On : 25 Aug 2023 12:51
 Operator : SY/MD
 Sample : 04138-01ME
 Misc : 5.54g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHQ5ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/28/2023
 Supervised By :Semsettin Yesilyurt 08/28/2023

Quant Time: Aug 26 00:52:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	273221	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	262834	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	134097	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	59991	35.084	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	70.160%	
7) Chloroethane-d5	1.526	69	37612	25.092	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	50.180%#	
11) 1,1-Dichloroethene-d2	2.040	65	28052	35.036	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	70.080%	
21) 2-Butanone-d5	3.815	46	113565	84.445	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	84.440%	
24) Chloroform-d	4.252	84	149855	40.096	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	80.200%	
26) 1,2-Dichloroethane-d4	4.944	65	102084	41.158	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	82.320%	
32) Benzene-d6	4.960	84	305838	42.644	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.280%	
36) 1,2-Dichloropropane-d6	5.992	67	103793	44.963	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	89.920%	
41) Toluene-d8	7.246	98	272409	41.222	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.440%	
43) trans-1,3-Dichloroprop...	7.558	79	51791	43.286	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.580%	
47) 2-Hexanone-d5	8.069	63	61042m	86.276	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	=	86.280%	
56) 1,1,2,2-Tetrachloroeth...	10.165	84	136024	45.599	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	11.570	152	104957	42.936	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	85.880%	
Target Compounds						
46) Tetrachloroethene	7.908	164	11084	8.173	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031930.D
Acq On : 25 Aug 2023 12:51
Operator : SY/MD
Sample : 04138-01ME
Misc : 5.54g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHQ5ME

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 08/28/2023
Supervised By :Semsettin Yesilyurt 08/28/2023

Quant Time: Aug 26 00:52:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

