

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031936.D
 Acq On : 25 Aug 2023 15:52
 Operator : SY/MD
 Sample : 04175-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR4

Quant Time: Aug 26 00:53:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	239552	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	232988	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	122026	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	55368	36.932	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.860%
7) Chloroethane-d5	1.532	69	53062	40.375	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.760%
11) 1,1-Dichloroethene-d2	2.063	65	26587	37.873	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.740%
21) 2-Butanone-d5	3.793	46	111458	94.527	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.530%
24) Chloroform-d	4.256	84	137628	42.000	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	4.947	65	93541	43.015	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.020%
32) Benzene-d6	4.966	84	280161	44.067	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.140%
36) 1,2-Dichloropropane-d6	5.995	67	95246	46.546	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.100%
41) Toluene-d8	7.246	98	246073	42.007	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.020%
43) trans-1,3-Dichloroprop...	7.558	79	45563	42.959	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.920%
47) 2-Hexanone-d5	8.030	63	56764	90.507	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.510%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	123642	46.758	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.520%
66) 1,2-Dichlorobenzene-d4	11.564	152	100630	45.238	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.480%
Target Compounds						
13) Acetone	2.118	43	8015	7.637	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031936.D
Acq On : 25 Aug 2023 15:52
Operator : SY/MD
Sample : 04175-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR4

Quant Time: Aug 26 00:53:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

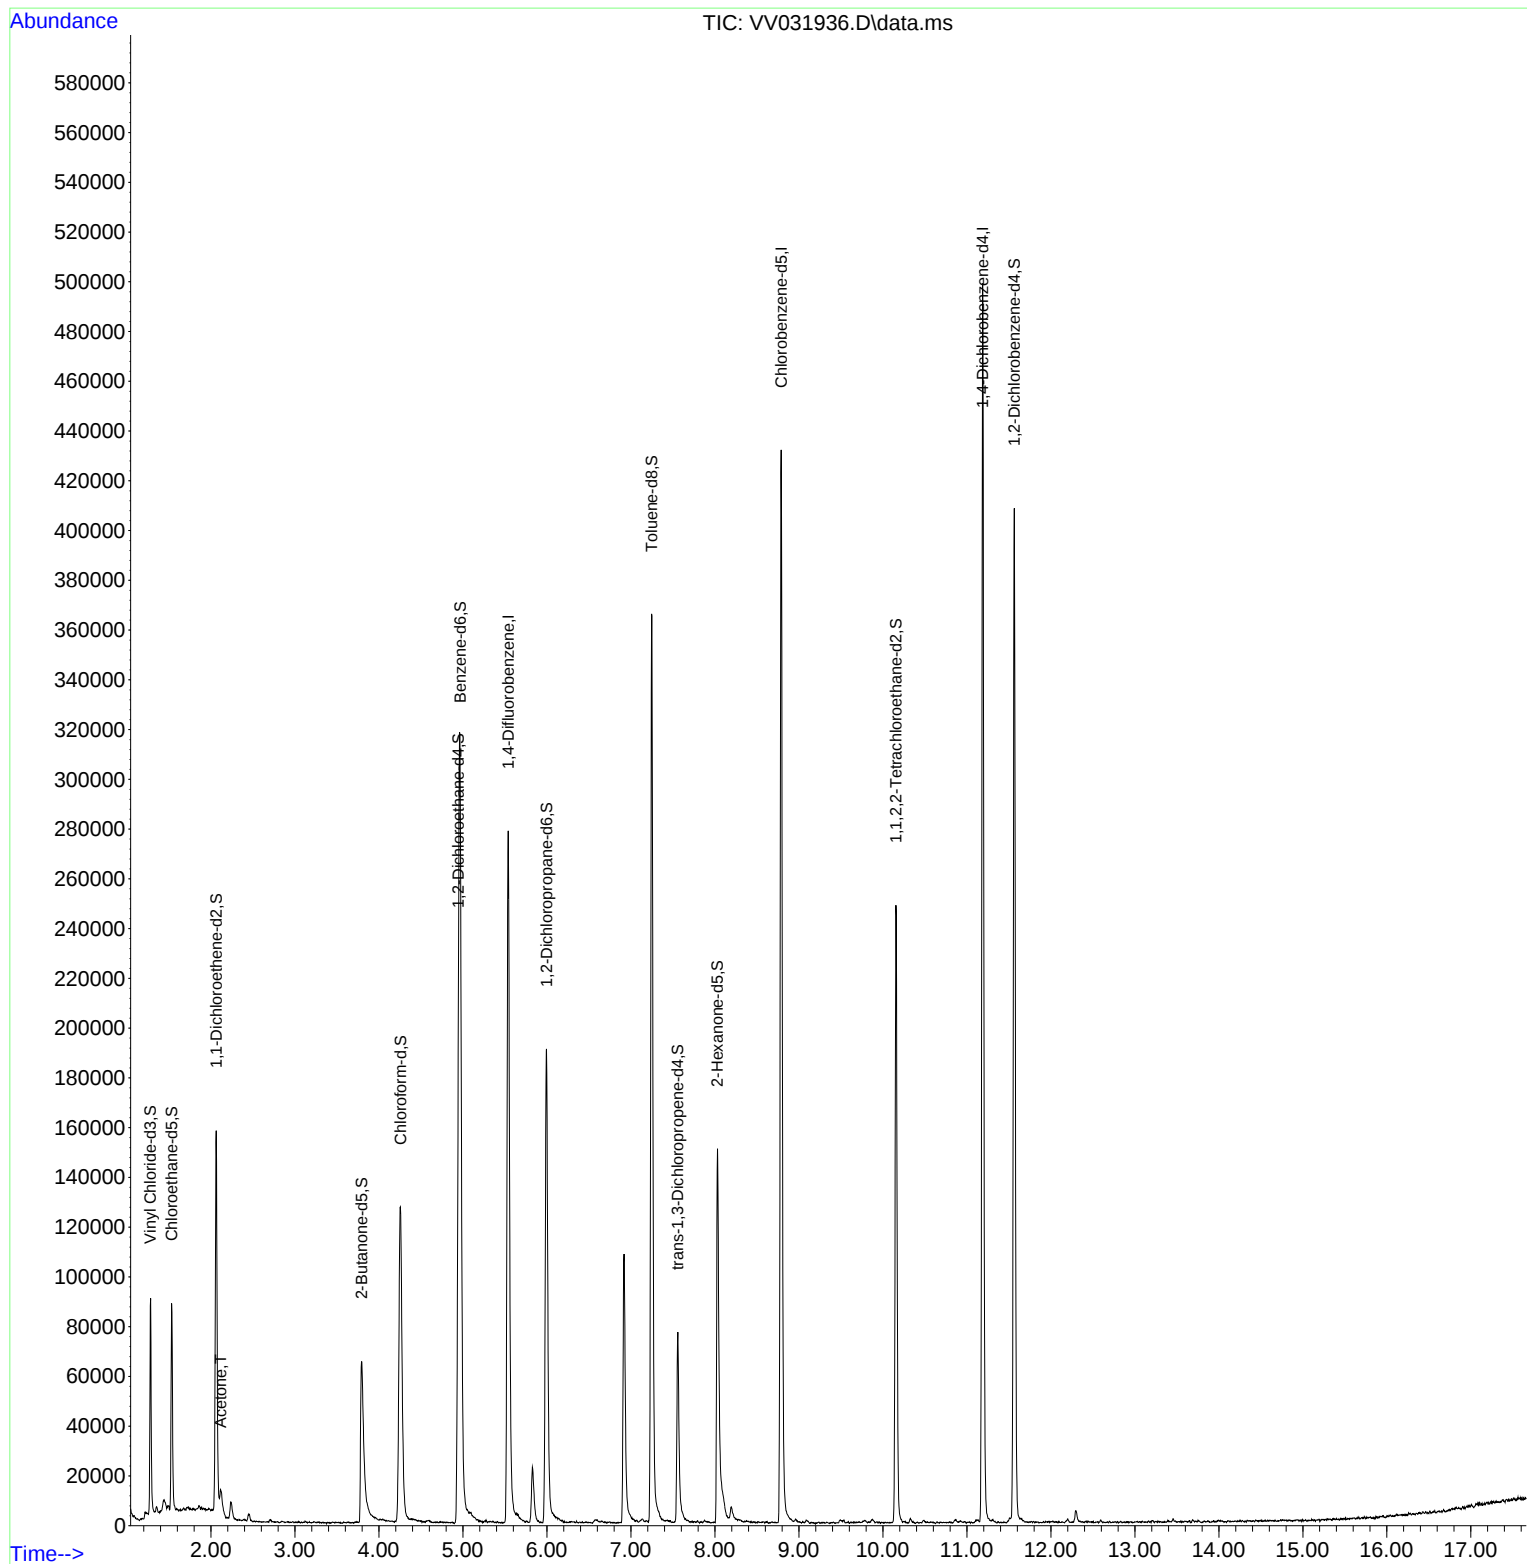

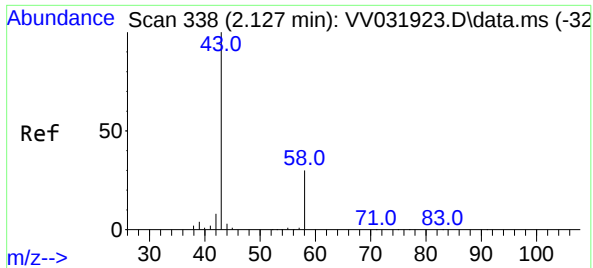

#13
Acetone
Concen: 7.637 ug/L
RT: 2.118 min Scan# 31
Delta R.T. -0.009 min
Lab File: VV031936.D
Acq: 25 Aug 2023 15:52

Instrument :
MSVOA_V
ClientSampleId :
EZYR4

Tgt Ion: 43 Resp: 8015
Ion Ratio Lower Upper
43 100
58 32.9 0.0 61.0

