

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031925.D
 Acq On : 25 Aug 2023 10:37
 Operator : SY/MD
 Sample : VV0825WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK382

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rBV	98419	104700	11.24%	1.440%
2	1.535	146	154	171	rVB	93577	113854	12.22%	1.566%
3	2.063	308	318	337	rBV	176456	258023	27.70%	3.548%
4	2.423	427	430	432	rBV3	551	311	0.03%	0.004%
5	2.445	432	437	439	rBV4	1959	1907	0.20%	0.026%
6	2.661	500	504	507	rBV3	411	302	0.03%	0.004%
7	2.706	515	518	519	rBV2	597	335	0.04%	0.005%
8	3.162	656	660	664	rBV3	526	435	0.05%	0.006%
9	3.420	735	740	744	rBV4	463	470	0.05%	0.006%
10	3.580	783	790	791	rBV3	537	557	0.06%	0.008%
11	3.690	822	824	829	rVB4	486	297	0.03%	0.004%
12	3.799	848	858	892	rBV	68997	210262	22.58%	2.892%
13	4.162	968	971	973	rBV2	554	331	0.04%	0.005%
14	4.252	983	999	1026	rBV	138998	359897	38.64%	4.950%
15	4.670	1125	1129	1134	rBV4	550	628	0.07%	0.009%
16	4.741	1147	1151	1158	rBV3	901	829	0.09%	0.011%
17	4.786	1162	1165	1170	rBV4	727	626	0.07%	0.009%
18	4.825	1174	1177	1184	rVB6	728	614	0.07%	0.008%
19	4.854	1184	1186	1190	rBV4	600	490	0.05%	0.007%
20	4.960	1203	1219	1251	rBV2	348607	931344	100.00%	12.808%
21	5.326	1327	1333	1337	rVV5	667	839	0.09%	0.012%
22	5.413	1356	1360	1362	rBV3	517	349	0.04%	0.005%
23	5.452	1370	1372	1378	rVB5	680	499	0.05%	0.007%
24	5.484	1378	1382	1383	rBV2	465	344	0.04%	0.005%
25	5.538	1386	1399	1427	rBV	289536	604691	64.93%	8.316%
26	5.828	1478	1489	1503	rBV3	18969	40336	4.33%	0.555%
27	5.992	1527	1540	1566	rBV	207551	433178	46.51%	5.957%
28	6.201	1601	1605	1607	rBV3	576	399	0.04%	0.005%
29	6.259	1621	1623	1630	rVB4	612	550	0.06%	0.008%
30	6.304	1634	1637	1640	rBV3	626	526	0.06%	0.007%
31	6.471	1685	1689	1693	rBV3	562	450	0.05%	0.006%
32	6.587	1713	1725	1729	rBV7	1297	2746	0.29%	0.038%
33	6.796	1787	1790	1792	rBV2	358	283	0.03%	0.004%
34	6.918	1816	1828	1846	rBV	118525	225673	24.23%	3.104%
35	7.246	1918	1930	1957	rBV	413808	742021	79.67%	10.205%
36	7.500	2007	2009	2013	rVB2	572	373	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031925.D
 Acq On : 25 Aug 2023 10:37
 Operator : SY/MD
 Sample : VV0825WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK382

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.558	2017	2027	2050	rBV	82131	153203	16.45%	2.107%
38	7.844	2112	2116	2120	rVB5	423	402	0.04%	0.006%
39	7.918	2136	2139	2142	rBV3	593	306	0.03%	0.004%
40	8.030	2164	2174	2211	rBV	162584	334175	35.88%	4.596%
41	8.365	2271	2278	2290	rVB6	1963	3847	0.41%	0.053%
42	8.445	2301	2303	2308	rVB6	585	490	0.05%	0.007%
43	8.606	2348	2353	2357	rVV4	506	524	0.06%	0.007%
44	8.702	2378	2383	2386	rBV4	436	389	0.04%	0.005%
45	8.722	2386	2389	2392	rVB2	492	357	0.04%	0.005%
46	8.744	2392	2396	2399	rBV5	831	706	0.08%	0.010%
47	8.789	2399	2410	2441	rBV	446711	751302	80.67%	10.332%
48	8.953	2459	2461	2468	rVB6	630	628	0.07%	0.009%
49	9.156	2521	2524	2526	rBV3	446	287	0.03%	0.004%
50	9.300	2564	2569	2572	rBV5	646	485	0.05%	0.007%
51	9.477	2622	2624	2628	rVB3	484	333	0.04%	0.005%
52	9.580	2651	2656	2660	rVB5	490	472	0.05%	0.006%
53	9.693	2689	2691	2694	rVB2	900	424	0.05%	0.006%
54	9.712	2694	2697	2702	rBV3	762	926	0.10%	0.013%
55	9.763	2708	2713	2718	rBV2	456	526	0.06%	0.007%
56	9.876	2746	2748	2755	rVB3	526	523	0.06%	0.007%
57	9.940	2764	2768	2772	rVB4	446	319	0.03%	0.004%
58	10.027	2791	2795	2800	rBV4	661	464	0.05%	0.006%
59	10.056	2800	2804	2806	rBV3	433	322	0.03%	0.004%
60	10.156	2821	2835	2857	rBV	265391	430497	46.22%	5.920%
61	10.262	2865	2868	2874	rBV3	475	511	0.05%	0.007%
62	10.294	2874	2878	2881	rVB2	463	343	0.04%	0.005%
63	10.332	2887	2890	2898	rVB3	880	679	0.07%	0.009%
64	10.468	2927	2932	2934	rBV2	317	304	0.03%	0.004%
65	10.490	2936	2939	2944	rVB2	657	513	0.06%	0.007%
66	10.519	2944	2948	2952	rBV4	597	631	0.07%	0.009%
67	10.564	2959	2962	2967	rVB4	720	509	0.05%	0.007%
68	10.615	2976	2978	2985	rVB4	628	550	0.06%	0.008%
69	10.651	2985	2989	2992	rBV3	348	341	0.04%	0.005%
70	10.860	3047	3054	3055	rBV3	685	693	0.07%	0.010%
71	10.992	3093	3095	3101	rVB3	583	598	0.06%	0.008%
72	11.017	3101	3103	3106	rBV	447	295	0.03%	0.004%
73	11.133	3131	3139	3140	rBV5	969	1106	0.12%	0.015%
74	11.143	3140	3142	3145	rVB3	645	284	0.03%	0.004%
75	11.188	3145	3156	3178	rBV	512383	804320	86.36%	11.062%
76	11.336	3200	3202	3206	rVB4	782	409	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031925.D
 Acq On : 25 Aug 2023 10:37
 Operator : SY/MD
 Sample : VV0825WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK382

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.368	3209	3212	3216	rBV4	644	416	0.04%	0.006%
78	11.564	3261	3273	3297	rBV	449079	711020	76.34%	9.778%
79	12.255	3482	3488	3491	rBV5	663	684	0.07%	0.009%
80	12.455	3545	3550	3553	rBV5	545	524	0.06%	0.007%
81	12.516	3566	3569	3572	rBV3	403	348	0.04%	0.005%
82	12.583	3588	3590	3591	rBV2	872	435	0.05%	0.006%
83	12.651	3609	3611	3616	rVV2	692	561	0.06%	0.008%
84	12.693	3621	3624	3630	rVB4	486	441	0.05%	0.006%
85	12.908	3689	3691	3697	rVB4	605	344	0.04%	0.005%
86	13.207	3779	3784	3790	rVB8	1596	2136	0.23%	0.029%
87	13.284	3806	3808	3814	rVB3	517	366	0.04%	0.005%
88	13.448	3851	3859	3869	rBV2	9096	15574	1.67%	0.214%
89	13.590	3900	3903	3906	rBV3	765	452	0.05%	0.006%
90	13.683	3927	3932	3933	rBV3	2136	1253	0.13%	0.017%
91	13.869	3988	3990	3994	rVB3	552	308	0.03%	0.004%
92	13.892	3994	3997	4000	rBV5	475	360	0.04%	0.005%
93	13.963	4017	4019	4024	rVB3	575	316	0.03%	0.004%
94	14.072	4050	4053	4056	rBV2	478	356	0.04%	0.005%
95	14.088	4056	4058	4064	rVB5	432	349	0.04%	0.005%
96	14.159	4078	4080	4083	rBV2	668	339	0.04%	0.005%
97	14.236	4102	4104	4106	rBV	463	279	0.03%	0.004%
98	14.387	4149	4151	4155	rBV2	421	324	0.03%	0.004%
99	14.847	4292	4294	4296	rBV2	685	299	0.03%	0.004%
100	15.049	4355	4357	4361	rBV4	543	387	0.04%	0.005%




Sum of corrected areas: 7271333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031925.D
Acq On : 25 Aug 2023 10:37
Operator : SY/MD
Sample : VV0825WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

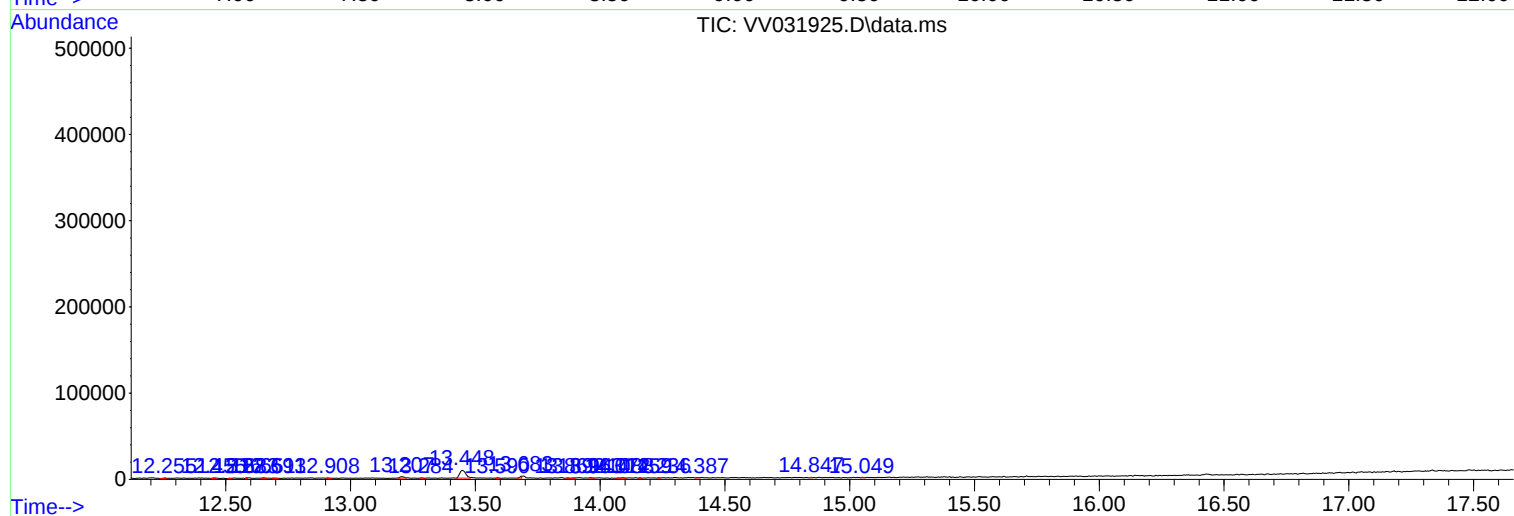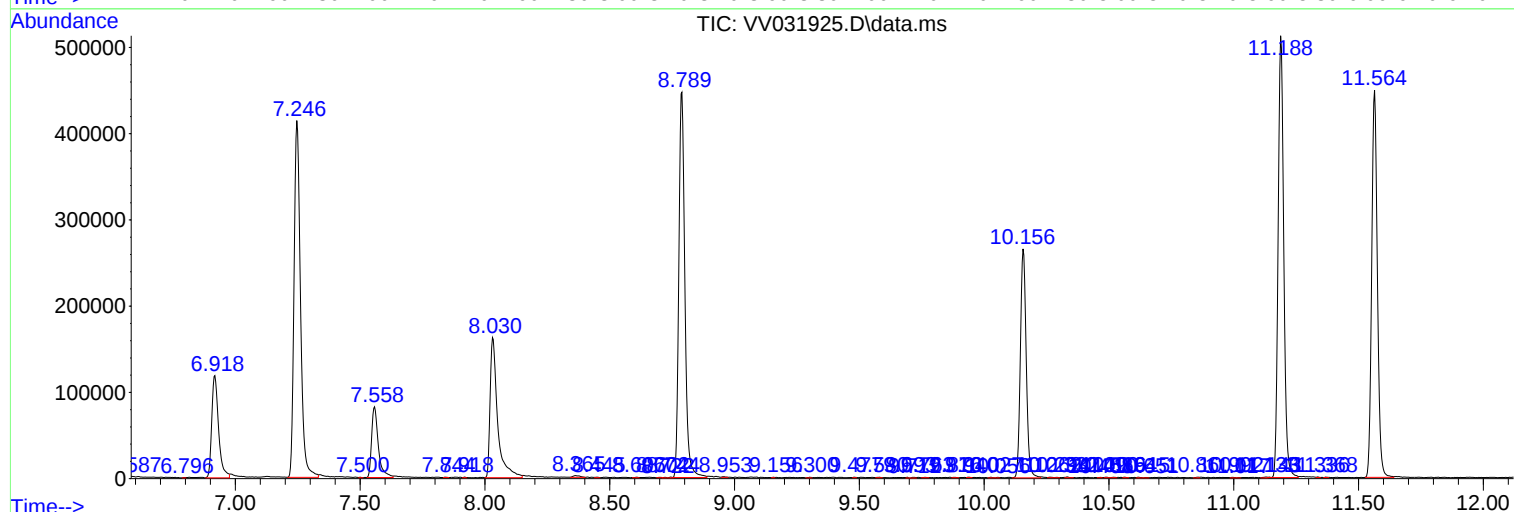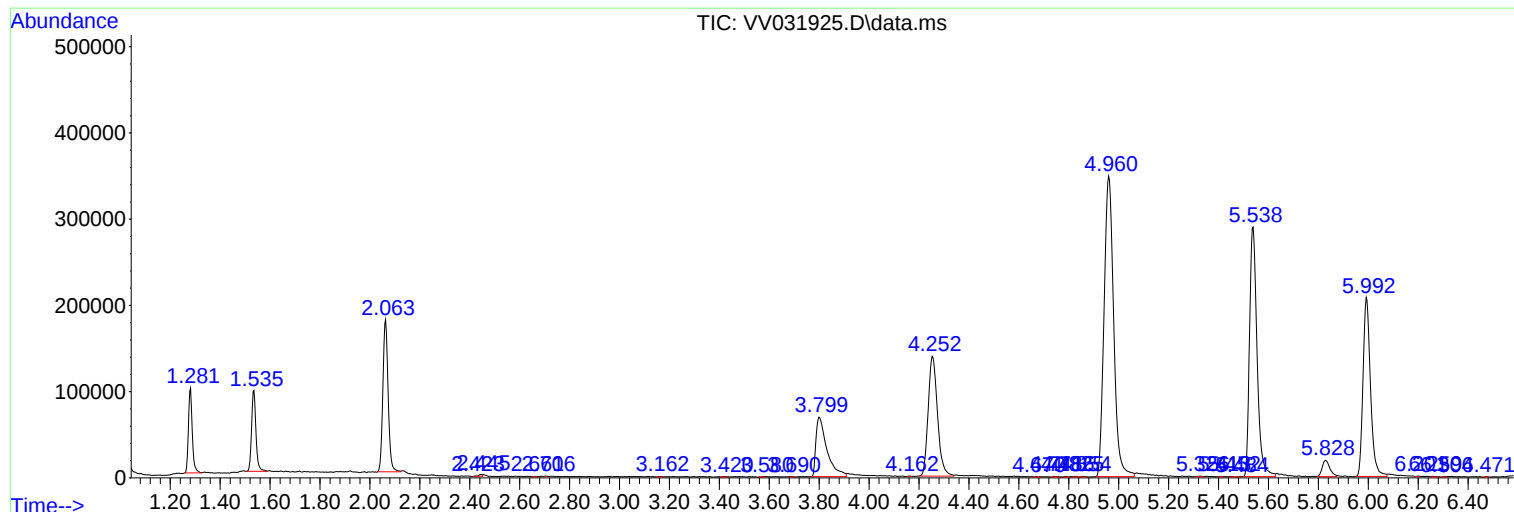

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031925.D
Acq On : 25 Aug 2023 10:37
Operator : SY/MD
Sample : VV0825WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031925.D
Acq On : 25 Aug 2023 10:37
Operator : SY/MD
Sample : VV0825WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------