

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031926.D
 Acq On : 25 Aug 2023 11:00
 Operator : SY/MD
 Sample : 04108-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	86665	91074	10.48%	1.351%
2	1.536	148	154	174	rVB	86159	102694	11.82%	1.523%
3	2.063	310	318	331	rVB	156378	221816	25.54%	3.290%
4	3.587	790	792	794	rBV3	316	195	0.02%	0.003%
5	3.748	837	842	844	rBV2	218	163	0.02%	0.002%
6	3.799	846	858	889	rBV	72267	217073	24.99%	3.220%
7	4.256	986	1000	1025	rVB	125662	321793	37.04%	4.773%
8	4.654	1122	1124	1127	rBV2	385	241	0.03%	0.004%
9	4.670	1127	1129	1131	rVB2	446	193	0.02%	0.003%
10	4.815	1171	1174	1176	rBV3	225	144	0.02%	0.002%
11	4.850	1182	1185	1188	rBV3	428	347	0.04%	0.005%
12	4.960	1203	1219	1253	rBV2	324673	868663	100.00%	12.886%
13	5.342	1333	1338	1342	rBV4	541	696	0.08%	0.010%
14	5.539	1387	1399	1425	rBV	266337	548533	63.15%	8.137%
15	5.831	1478	1490	1511	rVB2	17575	38619	4.45%	0.573%
16	5.992	1527	1540	1567	rBV	193109	407361	46.90%	6.043%
17	6.381	1658	1661	1665	rBV5	409	251	0.03%	0.004%
18	6.510	1699	1701	1702	rBV2	163	56	0.01%	0.001%
19	6.703	1757	1761	1763	rBV3	448	323	0.04%	0.005%
20	6.809	1791	1794	1797	rBV3	579	412	0.05%	0.006%
21	6.918	1817	1828	1851	rBV	111535	212395	24.45%	3.151%
22	7.246	1919	1930	1967	rBV	379847	683306	78.66%	10.136%
23	7.558	2017	2027	2048	rBV	77099	142698	16.43%	2.117%
24	7.870	2120	2124	2127	rBV4	814	628	0.07%	0.009%
25	7.915	2136	2138	2140	rBV2	400	152	0.02%	0.002%
26	7.969	2153	2155	2156	rBV	242	97	0.01%	0.001%
27	8.030	2165	2174	2213	rBV	163787	332565	38.28%	4.933%
28	8.609	2347	2354	2356	rBV4	525	584	0.07%	0.009%
29	8.638	2360	2363	2365	rBV3	402	247	0.03%	0.004%
30	8.657	2367	2369	2370	rBV2	455	194	0.02%	0.003%
31	8.706	2381	2384	2387	rBV3	537	336	0.04%	0.005%
32	8.789	2399	2410	2435	rBV	418417	694998	80.01%	10.310%
33	9.040	2486	2488	2491	rBV4	584	354	0.04%	0.005%
34	9.130	2512	2516	2519	rBV2	453	395	0.05%	0.006%
35	9.149	2519	2522	2523	rBV2	514	253	0.03%	0.004%
36	9.230	2544	2547	2550	rBV3	493	401	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031926.D
 Acq On : 25 Aug 2023 11:00
 Operator : SY/MD
 Sample : 04108-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	9.345	2578	2583	2584	rVB3	398	268	0.03%	0.004%
38	9.371	2588	2591	2592	rBV2	210	117	0.01%	0.002%
39	9.410	2601	2603	2607	rVB3	392	226	0.03%	0.003%
40	9.448	2611	2615	2618	rBV2	528	448	0.05%	0.007%
41	9.542	2641	2644	2650	rVB4	716	612	0.07%	0.009%
42	9.567	2650	2652	2654	rVV2	333	217	0.02%	0.003%
43	9.587	2654	2658	2662	rVV4	688	673	0.08%	0.010%
44	9.622	2666	2669	2674	rBV3	451	484	0.06%	0.007%
45	9.651	2676	2678	2681	rVB3	477	281	0.03%	0.004%
46	9.702	2693	2694	2695	rBV	254	83	0.01%	0.001%
47	9.770	2710	2715	2717	rBV2	471	417	0.05%	0.006%
48	9.796	2720	2723	2724	rBV2	400	163	0.02%	0.002%
49	9.841	2731	2737	2739	rBV4	636	653	0.08%	0.010%
50	9.876	2745	2748	2752	rBV3	492	373	0.04%	0.006%
51	9.921	2760	2762	2763	rBV	244	87	0.01%	0.001%
52	9.950	2769	2771	2772	rBV	324	139	0.02%	0.002%
53	10.098	2815	2817	2820	rBV2	408	322	0.04%	0.005%
54	10.156	2824	2835	2856	rVV	265144	419061	48.24%	6.216%
55	10.326	2886	2888	2891	rVB4	639	296	0.03%	0.004%
56	10.381	2902	2905	2908	rBV3	552	415	0.05%	0.006%
57	10.397	2908	2910	2912	rBV2	432	220	0.03%	0.003%
58	10.471	2928	2933	2934	rBV2	575	462	0.05%	0.007%
59	10.542	2954	2955	2956	rBV	354	109	0.01%	0.002%
60	10.580	2962	2967	2968	rBV2	649	533	0.06%	0.008%
61	10.725	3011	3012	3013	rBV	245	90	0.01%	0.001%
62	10.847	3046	3050	3051	rBV2	532	409	0.05%	0.006%
63	10.873	3054	3058	3061	rVV4	582	531	0.06%	0.008%
64	10.905	3065	3068	3071	rVB3	572	313	0.04%	0.005%
65	10.921	3071	3073	3075	rBV2	305	137	0.02%	0.002%
66	10.956	3082	3084	3087	rBB4	341	128	0.01%	0.002%
67	10.972	3087	3089	3094	rVB2	708	521	0.06%	0.008%
68	11.005	3094	3099	3100	rBV3	691	664	0.08%	0.010%
69	11.046	3109	3112	3116	rBV2	387	334	0.04%	0.005%
70	11.136	3137	3140	3144	rVB4	673	533	0.06%	0.008%
71	11.188	3144	3156	3180	rBV	473373	747484	86.05%	11.088%
72	11.368	3210	3212	3215	rVB2	581	303	0.03%	0.004%
73	11.493	3249	3251	3254	rBV4	498	285	0.03%	0.004%
74	11.564	3261	3273	3291	rBV	418970	664908	76.54%	9.863%
75	11.879	3368	3371	3372	rBV	353	229	0.03%	0.003%
76	12.124	3444	3447	3448	rBV2	474	297	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031926.D
Acq On : 25 Aug 2023 11:00
Operator : SY/MD
Sample : 04108-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M

Title : VOC Analysis

77	12.169	3459	3461	3467	rVB3	551	528	0.06%	0.008%
78	12.204	3467	3472	3475	rBV4	830	730	0.08%	0.011%
79	12.268	3490	3492	3494	rBV2	241	116	0.01%	0.002%
80	12.802	3657	3658	3661	rBV2	273	170	0.02%	0.003%
81	13.381	3835	3838	3840	rBV3	509	310	0.04%	0.005%
82	13.451	3855	3860	3870	rVB4	3101	4778	0.55%	0.071%
83	14.178	4082	4086	4089	rBV4	657	592	0.07%	0.009%




Sum of corrected areas: 6741299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031926.D
Acq On : 25 Aug 2023 11:00
Operator : SY/MD
Sample : 04108-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

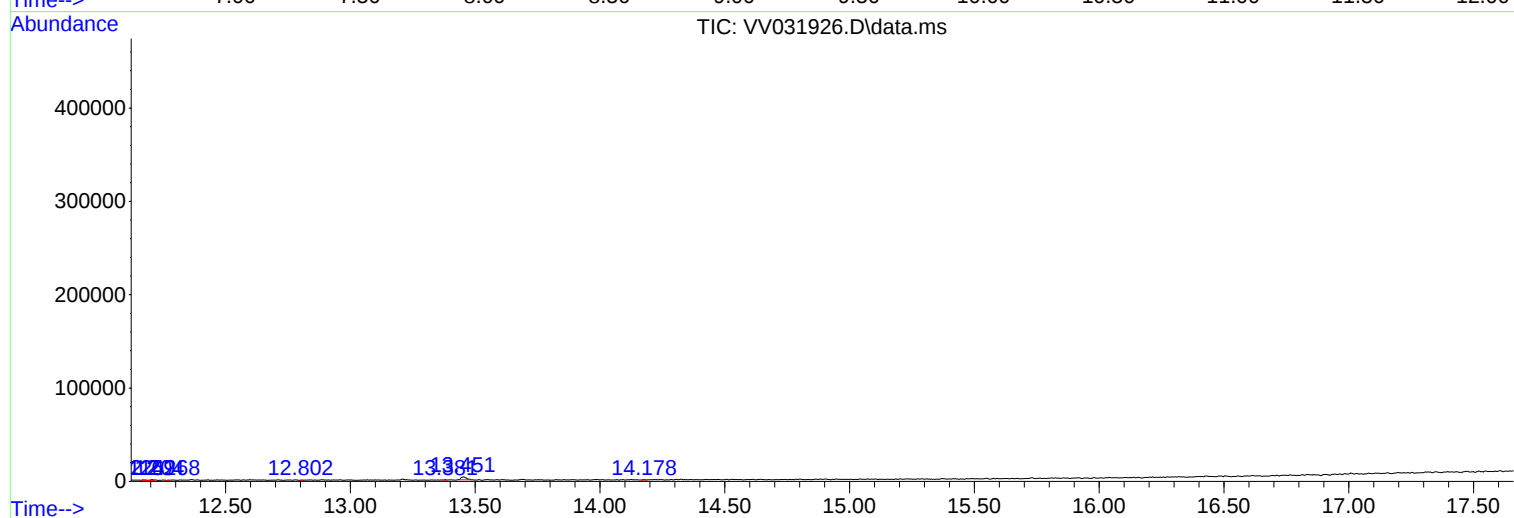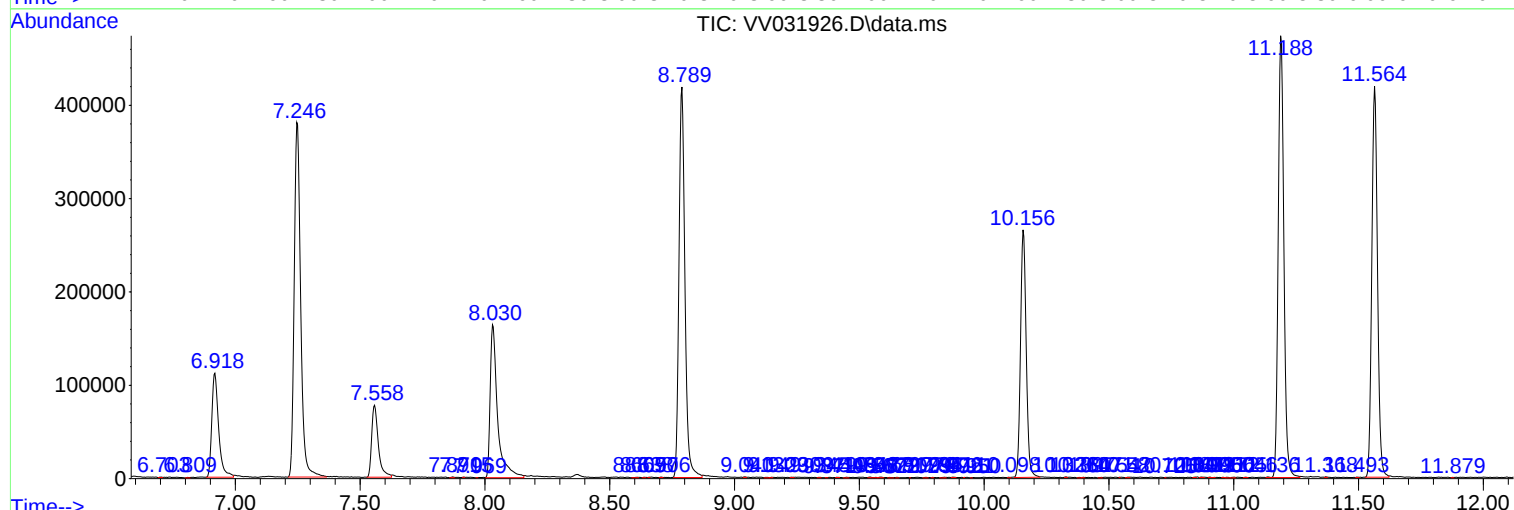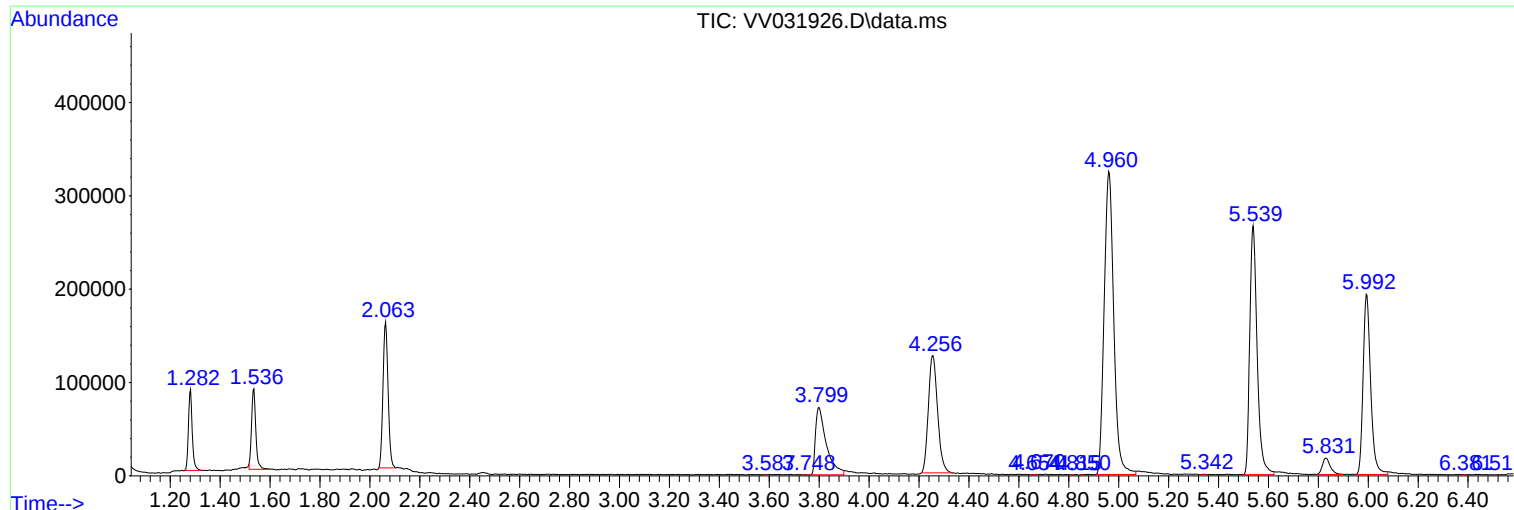

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031926.D
Acq On : 25 Aug 2023 11:00
Operator : SY/MD
Sample : 04108-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031926.D
Acq On : 25 Aug 2023 11:00
Operator : SY/MD
Sample : 04108-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc