

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031927.D
 Acq On : 25 Aug 2023 11:41
 Operator : SY/MD
 Sample : 04113-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BZYN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	86	rVB	94615	97451	10.62%	1.360%
2	1.536	147	154	167	rVB	90521	105487	11.49%	1.473%
3	2.060	309	317	331	rBV	171306	247419	26.96%	3.454%
4	3.053	624	626	629	rBV3	290	157	0.02%	0.002%
5	3.404	730	735	738	rBV4	402	439	0.05%	0.006%
6	3.420	738	740	742	rBV2	307	132	0.01%	0.002%
7	3.468	753	755	758	rVB2	519	294	0.03%	0.004%
8	3.539	775	777	781	rVB	394	192	0.02%	0.003%
9	3.561	781	784	786	rBV2	457	255	0.03%	0.004%
10	3.799	849	858	900	rBV	60092	196924	21.46%	2.749%
11	4.249	984	998	1027	rBV	135829	350901	38.23%	4.899%
12	4.629	1115	1116	1117	rBV	220	73	0.01%	0.001%
13	4.780	1160	1163	1164	rBV3	316	162	0.02%	0.002%
14	4.857	1184	1187	1189	rBV3	564	350	0.04%	0.005%
15	4.957	1202	1218	1248	rBV2	345947	917831	100.00%	12.813%
16	5.426	1361	1364	1365	rBV	373	253	0.03%	0.004%
17	5.468	1375	1377	1380	rBV2	474	284	0.03%	0.004%
18	5.535	1386	1398	1425	rBV	294811	608355	66.28%	8.493%
19	5.825	1480	1488	1510	rVB2	22550	47282	5.15%	0.660%
20	5.992	1527	1540	1563	rBV	204069	421600	45.93%	5.886%
21	6.227	1611	1613	1614	rBV	499	143	0.02%	0.002%
22	6.416	1669	1672	1673	rBV	421	243	0.03%	0.003%
23	6.529	1705	1707	1708	rBV2	391	129	0.01%	0.002%
24	6.789	1785	1788	1789	rBV2	324	132	0.01%	0.002%
25	6.915	1816	1827	1849	rBV	119611	224109	24.42%	3.129%
26	7.246	1918	1930	1968	rBV	410206	736462	80.24%	10.281%
27	7.555	2015	2026	2059	rBV	80988	153420	16.72%	2.142%
28	7.879	2115	2127	2138	rBV	13010	23893	2.60%	0.334%
29	7.941	2144	2146	2148	rBV2	430	216	0.02%	0.003%
30	8.031	2165	2174	2216	rBV	150140	318350	34.69%	4.444%
31	8.477	2311	2313	2314	rBV	494	186	0.02%	0.003%
32	8.580	2343	2345	2348	rVB3	507	199	0.02%	0.003%
33	8.596	2348	2350	2353	rVV2	484	272	0.03%	0.004%
34	8.616	2353	2356	2361	rVB4	471	375	0.04%	0.005%
35	8.661	2368	2370	2371	rBV	316	115	0.01%	0.002%
36	8.786	2397	2409	2438	rBV	458344	756540	82.43%	10.561%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031927.D
 Acq On : 25 Aug 2023 11:41
 Operator : SY/MD
 Sample : 04113-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BZYN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	9.082	2498	2501	2502	rBV2	523	278	0.03%	0.004%
38	9.156	2520	2524	2526	rBV3	462	285	0.03%	0.004%
39	9.214	2540	2542	2544	rBV2	362	138	0.02%	0.002%
40	9.262	2554	2557	2558	rBV2	398	229	0.02%	0.003%
41	9.494	2625	2629	2631	rBV3	557	455	0.05%	0.006%
42	9.506	2631	2633	2634	rBV2	358	128	0.01%	0.002%
43	9.542	2641	2644	2648	rBV3	373	397	0.04%	0.006%
44	9.612	2662	2666	2667	rBV	216	129	0.01%	0.002%
45	9.625	2667	2670	2673	rVV4	360	320	0.03%	0.004%
46	9.937	2763	2767	2768	rBV3	402	283	0.03%	0.004%
47	10.050	2800	2802	2806	rVB4	395	260	0.03%	0.004%
48	10.072	2807	2809	2812	rVB2	466	221	0.02%	0.003%
49	10.095	2812	2816	2819	rBV3	498	442	0.05%	0.006%
50	10.156	2824	2835	2852	rBV	253286	398852	43.46%	5.568%
51	10.329	2879	2889	2902	rVB2	17209	27720	3.02%	0.387%
52	10.407	2911	2913	2916	rVB4	686	353	0.04%	0.005%
53	10.458	2926	2929	2931	rBV2	545	363	0.04%	0.005%
54	10.522	2943	2949	2951	rBV4	644	565	0.06%	0.008%
55	10.584	2965	2968	2972	rBV3	482	415	0.05%	0.006%
56	10.715	3008	3009	3010	rVB3	321	62	0.01%	0.001%
57	10.809	3034	3038	3042	rBV	411	425	0.05%	0.006%
58	10.892	3062	3064	3066	rBV2	539	278	0.03%	0.004%
59	11.188	3145	3156	3176	rBV	531038	812693	88.54%	11.345%
60	11.564	3262	3273	3296	rVB	439255	691963	75.39%	9.660%
61	11.876	3368	3370	3373	rVB3	449	152	0.02%	0.002%
62	12.088	3433	3436	3438	rBV3	368	259	0.03%	0.004%
63	12.117	3441	3445	3447	rBV3	541	455	0.05%	0.006%
64	12.201	3461	3471	3483	rBV2	5212	9421	1.03%	0.132%
65	12.558	3576	3582	3584	rBV4	613	579	0.06%	0.008%
66	12.628	3602	3604	3607	rBV	450	294	0.03%	0.004%
67	12.680	3618	3620	3623	rBV3	494	240	0.03%	0.003%
68	12.808	3658	3660	3661	rBV2	272	96	0.01%	0.001%
69	12.947	3701	3703	3706	rBV3	577	467	0.05%	0.007%
70	13.011	3722	3723	3724	rBV	189	62	0.01%	0.001%
71	13.027	3724	3728	3734	rVB4	684	720	0.08%	0.010%
72	13.056	3735	3737	3739	rBV2	344	186	0.02%	0.003%
73	13.095	3748	3749	3750	rBV2	352	107	0.01%	0.001%
74	13.143	3758	3764	3767	rBV5	649	739	0.08%	0.010%
75	13.278	3802	3806	3808	rVB2	499	350	0.04%	0.005%
76	13.313	3813	3817	3820	rBV2	739	692	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031927.D
Acq On : 25 Aug 2023 11:41
Operator : SY/MD
Sample : 04113-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYN8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis

77	13.735	3947	3948	3950	rBV	248	141	0.02%	0.002%
78	14.056	4046	4048	4053	rBV3	572	370	0.04%	0.005%




Sum of corrected areas: 7163209

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031927.D
Acq On : 25 Aug 2023 11:41
Operator : SY/MD
Sample : 04113-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

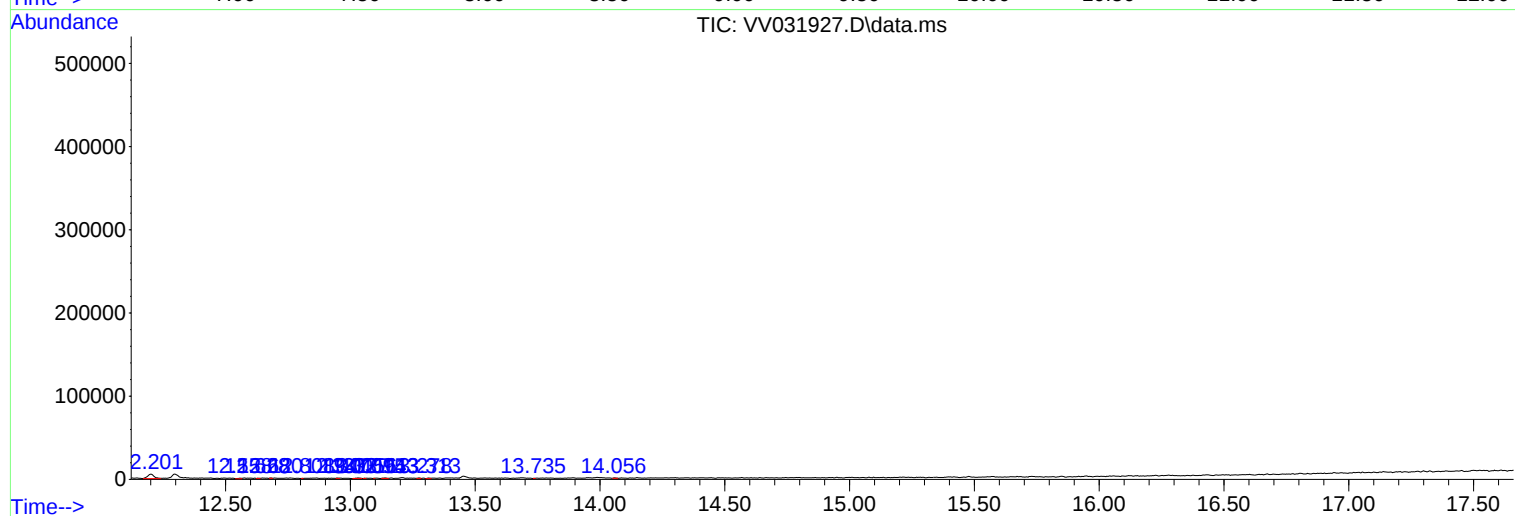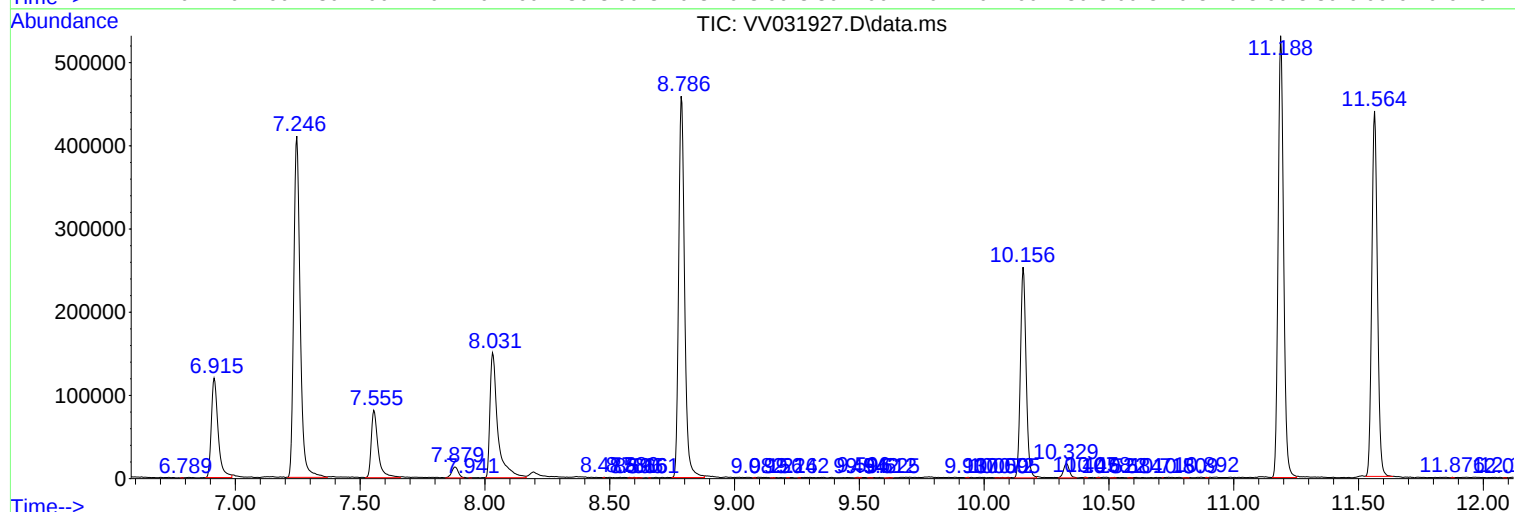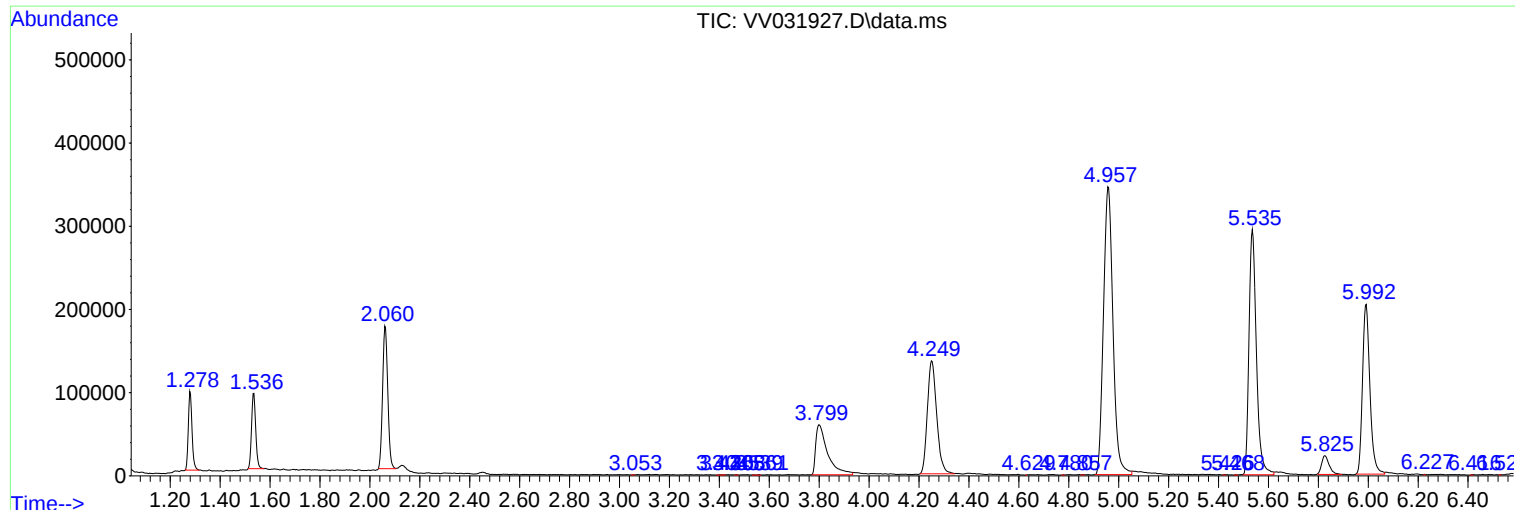

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031927.D
Acq On : 25 Aug 2023 11:41
Operator : SY/MD
Sample : 04113-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031927.D
Acq On : 25 Aug 2023 11:41
Operator : SY/MD
Sample : 04113-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc