

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031928.D
 Acq On : 25 Aug 2023 12:04
 Operator : SY/MD
 Sample : 04113-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BZYR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rVB	94842	100798	10.85%	1.412%
2	1.532	146	153	169	rVB	94356	112152	12.07%	1.571%
3	2.063	309	318	330	rBV	170327	246015	26.48%	3.447%
4	2.452	432	439	449	rVB3	3153	5429	0.58%	0.076%
5	2.802	544	548	551	rVB3	629	433	0.05%	0.006%
6	2.822	551	554	558	rBV3	537	439	0.05%	0.006%
7	2.934	587	589	594	rBV3	509	464	0.05%	0.007%
8	3.031	617	619	623	rVB4	370	269	0.03%	0.004%
9	3.297	698	702	706	rVV3	384	365	0.04%	0.005%
10	3.330	710	712	716	rBV3	329	290	0.03%	0.004%
11	3.404	730	735	736	rBV5	350	326	0.04%	0.005%
12	3.468	753	755	760	rVB4	489	277	0.03%	0.004%
13	3.529	770	774	777	rBV3	549	437	0.05%	0.006%
14	3.696	821	826	830	rVB5	511	498	0.05%	0.007%
15	3.796	848	857	891	rBV	67102	194027	20.88%	2.719%
16	4.252	982	999	1027	rBV	138892	360817	38.83%	5.056%
17	4.664	1123	1127	1130	rBV4	480	284	0.03%	0.004%
18	4.818	1171	1175	1178	rVB3	520	409	0.04%	0.006%
19	4.960	1200	1219	1249	rBV2	350276	929115	100.00%	13.018%
20	5.336	1334	1336	1337	rBV2	539	279	0.03%	0.004%
21	5.397	1353	1355	1358	rBV2	516	378	0.04%	0.005%
22	5.416	1358	1361	1365	rVV2	396	343	0.04%	0.005%
23	5.449	1366	1371	1373	rVB3	622	590	0.06%	0.008%
24	5.539	1386	1399	1426	rBV	279317	577131	62.12%	8.087%
25	5.828	1478	1489	1509	rBV2	22052	48620	5.23%	0.681%
26	5.902	1509	1512	1515	rVB4	766	520	0.06%	0.007%
27	5.992	1527	1540	1563	rBV	206848	431021	46.39%	6.039%
28	6.391	1660	1664	1667	rBV4	496	371	0.04%	0.005%
29	6.442	1677	1680	1683	rBV3	394	338	0.04%	0.005%
30	6.490	1691	1695	1699	rBV3	374	384	0.04%	0.005%
31	6.580	1713	1723	1728	rBV6	1981	3340	0.36%	0.047%
32	6.645	1741	1743	1745	rBV2	502	301	0.03%	0.004%
33	6.773	1777	1783	1788	rBV3	223	332	0.04%	0.005%
34	6.799	1788	1791	1795	rVV2	511	437	0.05%	0.006%
35	6.818	1795	1797	1801	rVB3	771	549	0.06%	0.008%
36	6.838	1801	1803	1807	rBV3	569	499	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031928.D
 Acq On : 25 Aug 2023 12:04
 Operator : SY/MD
 Sample : 04113-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BZYR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.918	1817	1828	1856	rBV	118297	229010	24.65%	3.209%
38	7.127	1885	1893	1898	rBV6	1373	2247	0.24%	0.031%
39	7.246	1919	1930	1967	rBV	406825	729722	78.54%	10.225%
40	7.558	2016	2027	2052	rBV	82071	151829	16.34%	2.127%
41	7.731	2076	2081	2082	rBV3	701	520	0.06%	0.007%
42	7.809	2103	2105	2108	rVB2	599	369	0.04%	0.005%
43	7.825	2108	2110	2115	rVB4	455	290	0.03%	0.004%
44	7.883	2115	2128	2139	rBV	7488	13544	1.46%	0.190%
45	8.030	2165	2174	2215	rBV	162392	331642	35.69%	4.647%
46	8.194	2219	2225	2238	rVB6	5467	10253	1.10%	0.144%
47	8.323	2264	2265	2270	rBV4	442	357	0.04%	0.005%
48	8.686	2371	2378	2380	rBV4	619	676	0.07%	0.009%
49	8.728	2389	2391	2395	rVB3	749	405	0.04%	0.006%
50	8.789	2397	2410	2435	rBV	426652	716744	77.14%	10.043%
51	9.063	2492	2495	2498	rVB3	880	597	0.06%	0.008%
52	9.226	2542	2546	2549	rBV3	365	371	0.04%	0.005%
53	9.390	2591	2597	2598	rBV4	326	294	0.03%	0.004%
54	9.493	2625	2629	2633	rVB4	356	312	0.03%	0.004%
55	9.657	2677	2680	2682	rBV	534	400	0.04%	0.006%
56	9.847	2737	2739	2743	rVB3	699	443	0.05%	0.006%
57	9.870	2743	2746	2749	rBV3	525	295	0.03%	0.004%
58	10.156	2824	2835	2854	rVV	261174	412877	44.44%	5.785%
59	10.329	2878	2889	2898	rBV3	10716	17923	1.93%	0.251%
60	10.416	2914	2916	2918	rBV2	401	270	0.03%	0.004%
61	10.477	2931	2935	2937	rBV3	736	611	0.07%	0.009%
62	10.680	2996	2998	3000	rBV2	554	295	0.03%	0.004%
63	10.898	3062	3066	3067	rBV2	523	371	0.04%	0.005%
64	10.908	3067	3069	3071	rVV2	563	320	0.03%	0.004%
65	11.008	3097	3100	3104	rBV4	543	381	0.04%	0.005%
66	11.107	3123	3131	3137	rBV9	1369	2418	0.26%	0.034%
67	11.188	3144	3156	3182	rBV	497725	763479	82.17%	10.698%
68	11.464	3237	3242	3244	rBV4	436	362	0.04%	0.005%
69	11.509	3247	3256	3261	rBV5	2570	4419	0.48%	0.062%
70	11.564	3262	3273	3292	rVB	443442	694866	74.79%	9.736%
71	11.693	3310	3313	3316	rBV3	634	411	0.04%	0.006%
72	11.741	3324	3328	3331	rBV4	391	349	0.04%	0.005%
73	12.008	3405	3411	3416	rBV5	490	662	0.07%	0.009%
74	12.140	3448	3452	3454	rBV3	443	318	0.03%	0.004%
75	12.201	3464	3471	3483	rVB3	3635	5807	0.63%	0.081%
76	12.297	3492	3501	3511	rBV7	6037	10231	1.10%	0.143%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031928.D
 Acq On : 25 Aug 2023 12:04
 Operator : SY/MD
 Sample : 04113-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BZYR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	12.455	3545	3550	3553	rVB4	571	449	0.05%	0.006%
78	12.480	3553	3558	3562	rVB5	511	570	0.06%	0.008%
79	12.564	3579	3584	3585	rBV2	585	374	0.04%	0.005%
80	12.677	3616	3619	3624	rVB3	863	734	0.08%	0.010%
81	12.702	3624	3627	3631	rBV3	584	593	0.06%	0.008%
82	12.818	3661	3663	3672	rVB4	667	870	0.09%	0.012%
83	12.921	3692	3695	3698	rBV4	569	525	0.06%	0.007%
84	12.953	3703	3705	3709	rVV3	402	301	0.03%	0.004%
85	13.088	3745	3747	3750	rBV3	420	281	0.03%	0.004%
86	13.140	3761	3763	3769	rVB5	405	305	0.03%	0.004%
87	13.213	3780	3786	3791	rBV7	589	667	0.07%	0.009%
88	13.390	3839	3841	3845	rVB4	657	450	0.05%	0.006%
89	13.451	3855	3860	3869	rVB6	1065	1288	0.14%	0.018%
90	13.532	3883	3885	3889	rVB3	684	412	0.04%	0.006%
91	13.554	3889	3892	3895	rBV3	493	412	0.04%	0.006%
92	13.728	3943	3946	3950	rVB6	608	412	0.04%	0.006%
93	13.898	3996	3999	4002	rBV	466	339	0.04%	0.005%
94	13.969	4018	4021	4022	rBV2	502	320	0.03%	0.004%
95	13.985	4024	4026	4029	rVB2	736	463	0.05%	0.006%
96	14.149	4075	4077	4081	rBV4	484	371	0.04%	0.005%
97	14.541	4197	4199	4203	rBV4	600	304	0.03%	0.004%
98	14.619	4218	4223	4225	rBV4	531	485	0.05%	0.007%
99	14.834	4287	4290	4294	rBV3	721	604	0.07%	0.008%
100	15.316	4437	4440	4441	rBV2	622	430	0.05%	0.006%




Sum of corrected areas: 7136926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031928.D
Acq On : 25 Aug 2023 12:04
Operator : SY/MD
Sample : 04113-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

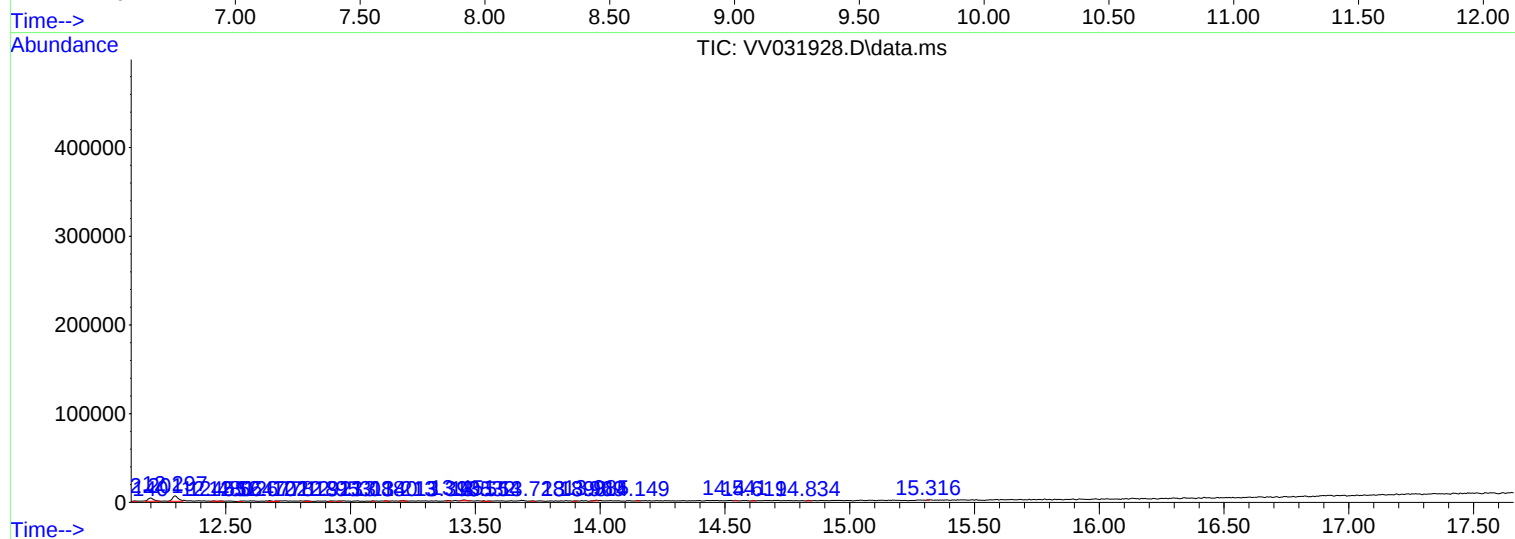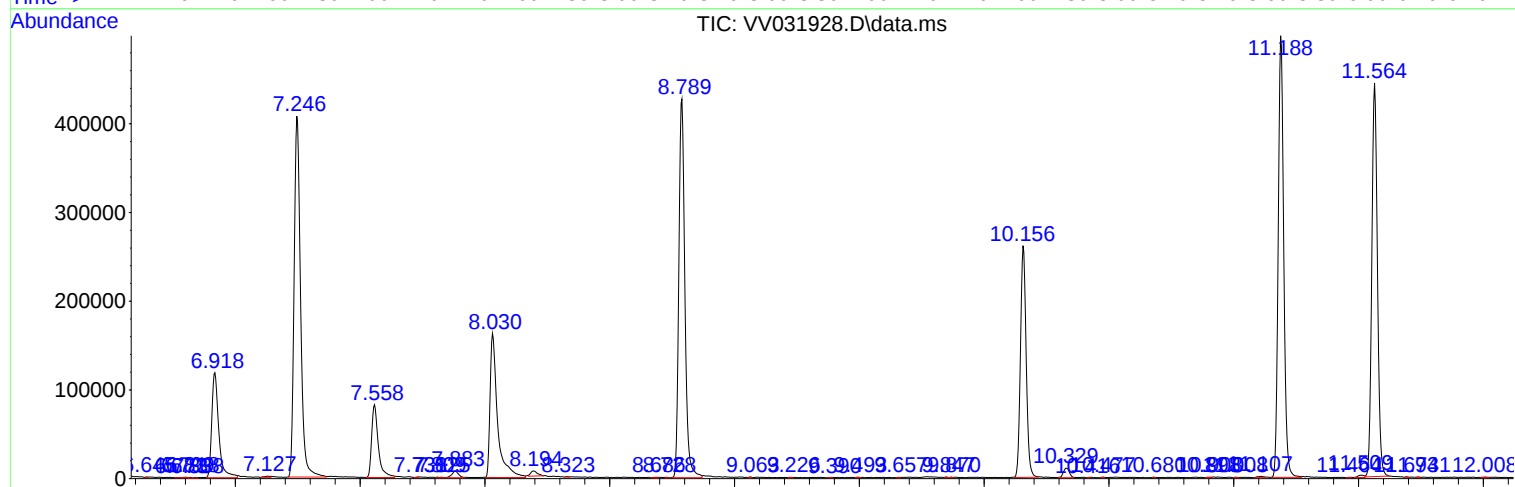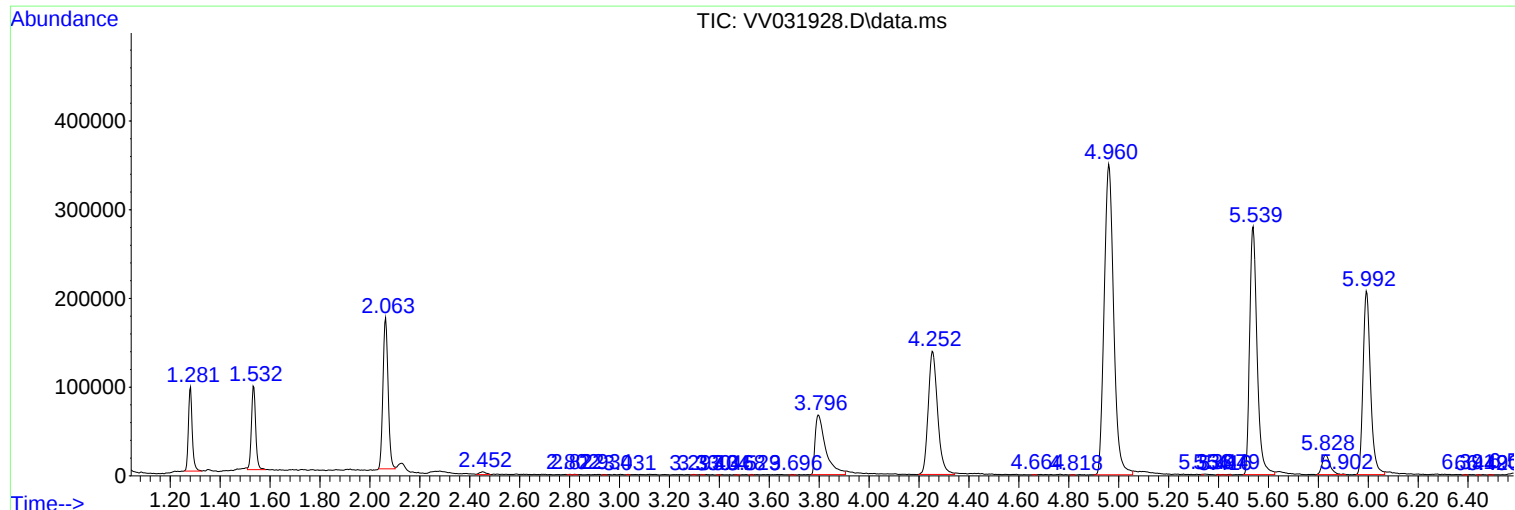

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031928.D
Acq On : 25 Aug 2023 12:04
Operator : SY/MD
Sample : 04113-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031928.D
Acq On : 25 Aug 2023 12:04
Operator : SY/MD
Sample : 04113-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BZYR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc