

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031934.D
 Acq On : 25 Aug 2023 14:28
 Operator : SY/MD
 Sample : 04113-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	86	rVB	86323	90880	10.25%	1.323%
2	1.532	147	153	168	rVB	87476	103965	11.73%	1.513%
3	2.063	309	318	331	rBV	162773	234866	26.50%	3.419%
4	2.500	452	454	457	rBV2	612	292	0.03%	0.004%
5	2.719	520	522	527	rVB5	626	436	0.05%	0.006%
6	3.137	650	652	653	rBV2	310	134	0.02%	0.002%
7	3.233	680	682	685	rVB4	706	317	0.04%	0.005%
8	3.262	688	691	692	rVV3	323	179	0.02%	0.003%
9	3.281	695	697	701	rVB4	704	430	0.05%	0.006%
10	3.301	701	703	705	rBV2	220	143	0.02%	0.002%
11	3.416	737	739	742	rBV3	250	186	0.02%	0.003%
12	3.529	770	774	777	rBV3	500	444	0.05%	0.006%
13	3.677	815	820	823	rBV3	478	410	0.05%	0.006%
14	3.719	830	833	837	rBV3	541	550	0.06%	0.008%
15	3.793	845	856	885	rBV	66365	191195	21.57%	2.783%
16	4.256	986	1000	1027	rVB2	132059	332500	37.51%	4.840%
17	4.529	1080	1085	1086	rBV3	475	369	0.04%	0.005%
18	4.696	1133	1137	1139	rBV2	385	271	0.03%	0.004%
19	4.738	1145	1150	1156	rBV5	534	769	0.09%	0.011%
20	4.767	1156	1159	1162	rBV3	616	405	0.05%	0.006%
21	4.815	1170	1174	1179	rBV4	378	427	0.05%	0.006%
22	4.844	1179	1183	1186	rVB4	360	243	0.03%	0.004%
23	4.860	1186	1188	1191	rBV3	474	335	0.04%	0.005%
24	4.899	1196	1200	1201	rBV3	338	254	0.03%	0.004%
25	4.960	1202	1219	1248	rBV2	331634	886436	100.00%	12.903%
26	5.323	1328	1332	1334	rBV5	658	468	0.05%	0.007%
27	5.378	1346	1349	1353	rBV4	519	324	0.04%	0.005%
28	5.452	1370	1372	1374	rBV2	307	151	0.02%	0.002%
29	5.477	1378	1380	1382	rBV2	243	172	0.02%	0.003%
30	5.539	1387	1399	1426	rBV	285259	584622	65.95%	8.510%
31	5.828	1478	1489	1510	rBV2	17092	38118	4.30%	0.555%
32	5.992	1527	1540	1565	rBV	196651	415515	46.87%	6.048%
33	6.317	1640	1641	1648	rVB5	599	626	0.07%	0.009%
34	6.352	1648	1652	1654	rBV3	442	364	0.04%	0.005%
35	6.384	1660	1662	1666	rBV4	613	444	0.05%	0.006%
36	6.413	1668	1671	1674	rBV3	472	362	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031934.D
 Acq On : 25 Aug 2023 14:28
 Operator : SY/MD
 Sample : 04113-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.474	1686	1690	1692	rBV4	462	276	0.03%	0.004%
38	6.567	1712	1719	1720	rBV5	1389	1197	0.14%	0.017%
39	6.725	1766	1768	1770	rBV2	471	297	0.03%	0.004%
40	6.776	1780	1784	1787	rBV5	750	528	0.06%	0.008%
41	6.815	1793	1796	1797	rBV	268	161	0.02%	0.002%
42	6.834	1800	1802	1805	rBV3	331	184	0.02%	0.003%
43	6.876	1813	1815	1816	rBV	302	136	0.02%	0.002%
44	6.918	1817	1828	1846	rBV	112635	210800	23.78%	3.068%
45	7.249	1919	1931	1970	rBV	388663	704758	79.50%	10.259%
46	7.516	2012	2014	2016	rVB2	393	132	0.01%	0.002%
47	7.558	2017	2027	2057	rVV	78487	145448	16.41%	2.117%
48	7.815	2106	2107	2114	rVB4	513	547	0.06%	0.008%
49	7.850	2114	2118	2119	rBV2	536	398	0.04%	0.006%
50	7.934	2141	2144	2145	rBV	376	203	0.02%	0.003%
51	8.030	2165	2174	2218	rBV	149737	304898	34.40%	4.438%
52	8.448	2302	2304	2307	rVB2	315	182	0.02%	0.003%
53	8.638	2361	2363	2366	rBV2	355	274	0.03%	0.004%
54	8.667	2370	2372	2374	rBV2	435	295	0.03%	0.004%
55	8.741	2393	2395	2398	rBV3	518	319	0.04%	0.005%
56	8.789	2398	2410	2438	rBV	441797	732646	82.65%	10.664%
57	9.008	2471	2478	2482	rBV5	782	894	0.10%	0.013%
58	9.053	2491	2492	2495	rBV2	626	276	0.03%	0.004%
59	9.117	2510	2512	2514	rBV2	383	210	0.02%	0.003%
60	9.165	2523	2527	2529	rVV4	453	421	0.05%	0.006%
61	9.278	2558	2562	2566	rBV4	661	628	0.07%	0.009%
62	9.384	2592	2595	2598	rBV3	505	387	0.04%	0.006%
63	9.419	2603	2606	2612	rVV5	653	583	0.07%	0.008%
64	9.448	2612	2615	2619	rVV3	509	406	0.05%	0.006%
65	9.757	2708	2711	2714	rBV3	500	406	0.05%	0.006%
66	9.799	2721	2724	2726	rBV3	270	162	0.02%	0.002%
67	9.837	2732	2736	2738	rBV2	538	307	0.03%	0.004%
68	10.034	2795	2797	2799	rBV	390	232	0.03%	0.003%
69	10.156	2824	2835	2859	rVB	262680	412100	46.49%	5.999%
70	10.371	2898	2902	2904	rVB2	382	227	0.03%	0.003%
71	10.452	2924	2927	2929	rBV2	350	205	0.02%	0.003%
72	10.471	2930	2933	2936	rVB3	503	335	0.04%	0.005%
73	10.525	2945	2950	2952	rBV2	443	385	0.04%	0.006%
74	10.661	2987	2992	2995	rBV4	545	593	0.07%	0.009%
75	10.770	3023	3026	3027	rBV2	272	147	0.02%	0.002%
76	10.805	3034	3037	3039	rBV2	308	164	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031934.D
 Acq On : 25 Aug 2023 14:28
 Operator : SY/MD
 Sample : 04113-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.831	3042	3045	3047	rBV2	365	201	0.02%	0.003%
78	10.850	3047	3051	3053	rVV2	372	277	0.03%	0.004%
79	10.895	3063	3065	3069	rVB	423	215	0.02%	0.003%
80	10.956	3078	3084	3086	rBV4	465	442	0.05%	0.006%
81	10.998	3094	3097	3100	rBV2	394	271	0.03%	0.004%
82	11.120	3133	3135	3136	rBV3	419	167	0.02%	0.002%
83	11.136	3139	3140	3142	rBV2	342	158	0.02%	0.002%
84	11.188	3145	3156	3175	rBV	498751	775994	87.54%	11.295%
85	11.371	3211	3213	3215	rVB	376	135	0.02%	0.002%
86	11.564	3261	3273	3291	rBV	420252	676784	76.35%	9.851%
87	11.767	3330	3336	3340	rBV4	578	603	0.07%	0.009%
88	12.172	3458	3462	3464	rBV5	534	350	0.04%	0.005%
89	12.323	3507	3509	3511	rBV3	369	158	0.02%	0.002%
90	12.535	3570	3575	3576	rBV4	676	616	0.07%	0.009%
91	12.554	3580	3581	3584	rBV2	433	262	0.03%	0.004%
92	12.593	3590	3593	3594	rBV2	455	299	0.03%	0.004%
93	12.699	3624	3626	3632	rVB4	360	333	0.04%	0.005%
94	12.744	3636	3640	3644	rBV4	398	414	0.05%	0.006%
95	12.779	3649	3651	3654	rBV3	561	297	0.03%	0.004%
96	13.374	3833	3836	3838	rBV3	578	443	0.05%	0.006%
97	13.448	3857	3859	3861	rBV2	522	229	0.03%	0.003%
98	13.512	3877	3879	3882	rBV	379	190	0.02%	0.003%
99	13.683	3930	3932	3935	rBV2	604	279	0.03%	0.004%
100	13.747	3949	3952	3955	rBV4	662	501	0.06%	0.007%




Sum of corrected areas: 6869967

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031934.D
Acq On : 25 Aug 2023 14:28
Operator : SY/MD
Sample : 04113-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

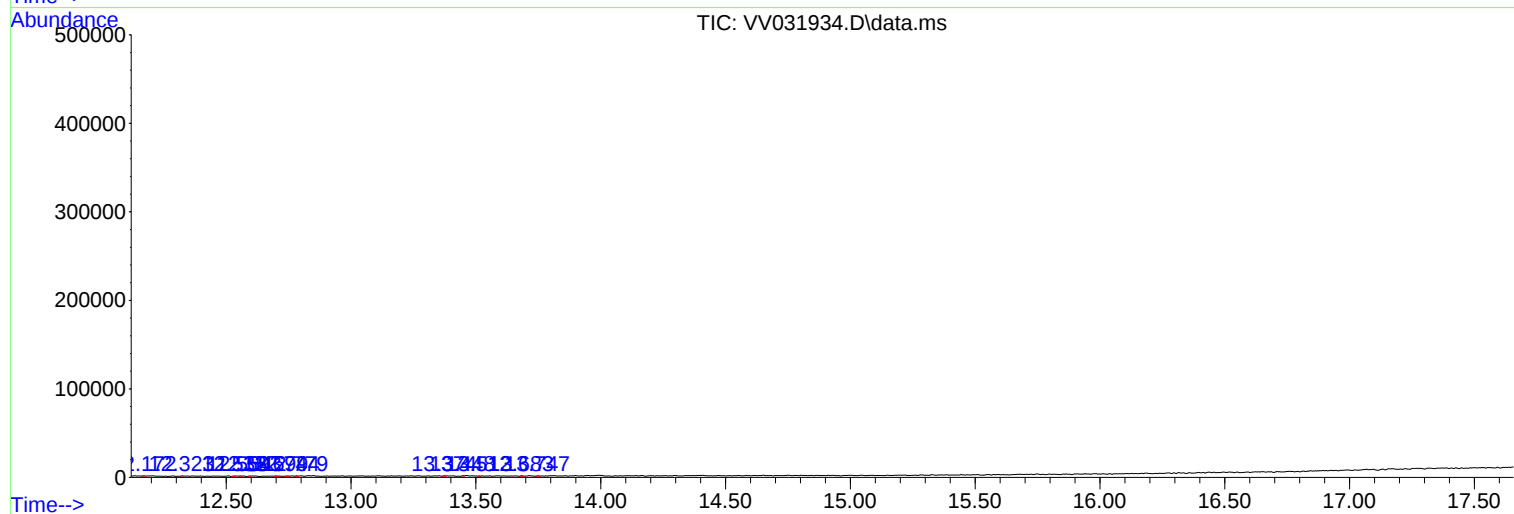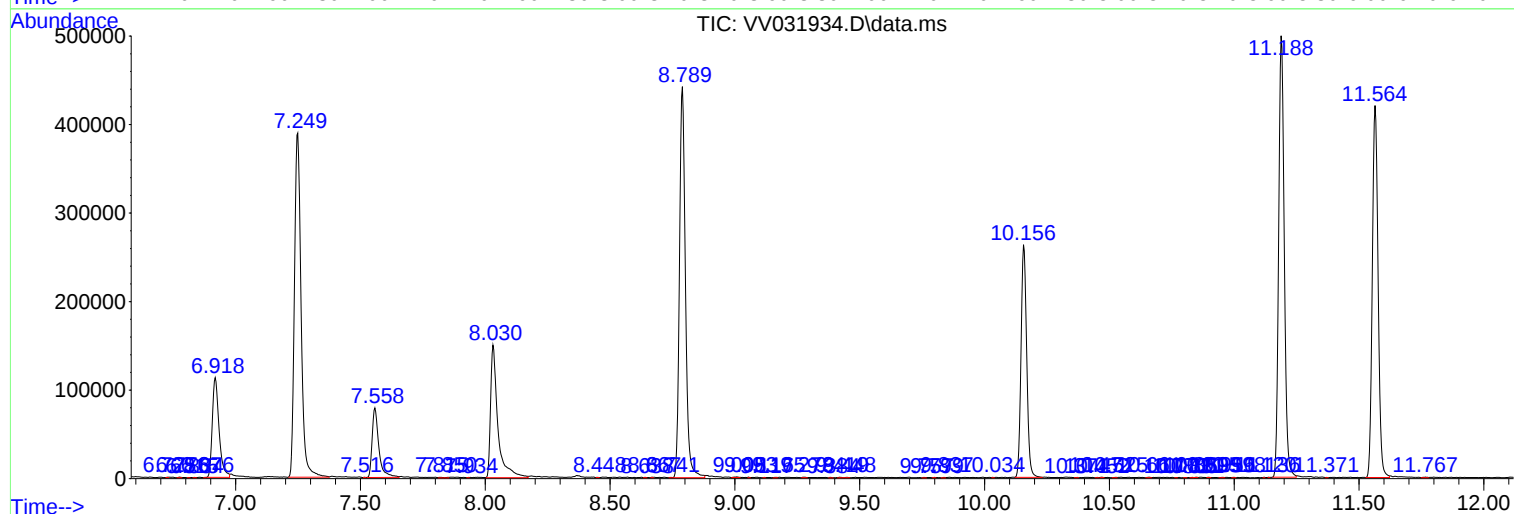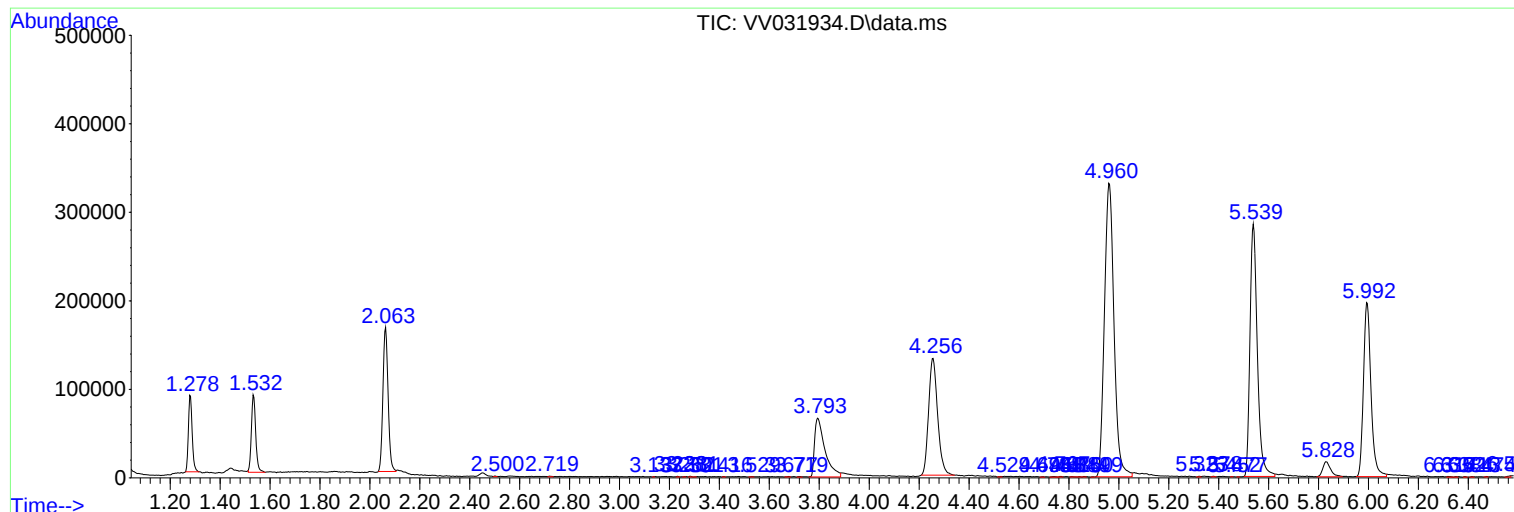

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031934.D
Acq On : 25 Aug 2023 14:28
Operator : SY/MD
Sample : 04113-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031934.D
Acq On : 25 Aug 2023 14:28
Operator : SY/MD
Sample : 04113-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
