

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031935.D
 Acq On : 25 Aug 2023 15:30
 Operator : SY/MD
 Sample : 04175-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	88484	93907	10.61%	1.348%
2	1.532	147	153	168	rVB	91196	108284	12.23%	1.554%
3	2.060	309	317	330	rBV	161033	229436	25.92%	3.294%
4	2.696	512	515	518	rBV3	538	343	0.04%	0.005%
5	2.831	555	557	558	rBV2	389	124	0.01%	0.002%
6	3.069	629	631	634	rBV3	344	157	0.02%	0.002%
7	3.088	634	637	640	rVB3	314	174	0.02%	0.002%
8	3.310	705	706	710	rVB2	595	281	0.03%	0.004%
9	3.420	735	740	744	rBV3	546	629	0.07%	0.009%
10	3.545	777	779	780	rBV	301	123	0.01%	0.002%
11	3.661	812	815	817	rBV3	522	293	0.03%	0.004%
12	3.674	817	819	821	rVV2	253	131	0.01%	0.002%
13	3.754	842	844	847	rBV2	344	216	0.02%	0.003%
14	3.793	847	856	891	rBV	62134	182036	20.56%	2.613%
15	4.252	985	999	1023	rVB	132005	338788	38.27%	4.864%
16	4.619	1111	1113	1115	rBV3	306	109	0.01%	0.002%
17	4.667	1126	1128	1131	rBV3	464	277	0.03%	0.004%
18	4.703	1138	1139	1142	rBV2	364	153	0.02%	0.002%
19	4.738	1147	1150	1152	rBV3	514	330	0.04%	0.005%
20	4.844	1181	1183	1188	rVB4	601	422	0.05%	0.006%
21	4.870	1188	1191	1193	rBV2	383	215	0.02%	0.003%
22	4.883	1193	1195	1199	rVB3	548	378	0.04%	0.005%
23	4.957	1199	1218	1247	rBV2	334343	885209	100.00%	12.708%
24	5.397	1353	1355	1357	rBV2	345	201	0.02%	0.003%
25	5.423	1360	1363	1365	rBV3	562	341	0.04%	0.005%
26	5.535	1385	1398	1429	rBV	297190	615303	69.51%	8.833%
27	5.825	1477	1488	1509	rBV2	21668	46959	5.30%	0.674%
28	5.992	1526	1540	1562	rBV	196157	415467	46.93%	5.964%
29	6.239	1612	1617	1621	rBV5	758	651	0.07%	0.009%
30	6.420	1669	1673	1677	rBV5	437	407	0.05%	0.006%
31	6.558	1712	1716	1717	rBV2	862	605	0.07%	0.009%
32	6.870	1810	1813	1817	rBV2	323	235	0.03%	0.003%
33	6.915	1817	1827	1851	rBV	113585	217177	24.53%	3.118%
34	7.246	1918	1930	1959	rBV	384733	693266	78.32%	9.952%
35	7.516	2010	2014	2016	rBV3	492	294	0.03%	0.004%
36	7.555	2016	2026	2057	rBV	78729	147470	16.66%	2.117%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031935.D
 Acq On : 25 Aug 2023 15:30
 Operator : SY/MD
 Sample : 04175-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.751	2084	2087	2090	rBV4	491	451	0.05%	0.006%
38	7.796	2096	2101	2104	rBV3	574	528	0.06%	0.008%
39	7.953	2148	2150	2152	rBV	304	166	0.02%	0.002%
40	7.963	2152	2153	2154	rBV	342	102	0.01%	0.001%
41	8.030	2165	2174	2213	rBV	150411	307733	34.76%	4.418%
42	8.452	2303	2305	2308	rBV3	303	124	0.01%	0.002%
43	8.519	2323	2326	2327	rBV2	629	301	0.03%	0.004%
44	8.641	2359	2364	2366	rBV5	441	458	0.05%	0.007%
45	8.744	2392	2396	2398	rBB2	511	294	0.03%	0.004%
46	8.786	2398	2409	2437	rBV	457808	762146	86.10%	10.941%
47	9.011	2471	2479	2484	rBV7	953	1412	0.16%	0.020%
48	9.079	2495	2500	2501	rBV4	536	437	0.05%	0.006%
49	9.313	2571	2573	2577	rVB2	370	198	0.02%	0.003%
50	9.342	2580	2582	2584	rBV3	315	163	0.02%	0.002%
51	9.365	2587	2589	2591	rBV2	497	271	0.03%	0.004%
52	9.445	2611	2614	2618	rVB3	533	370	0.04%	0.005%
53	9.471	2619	2622	2625	rBV3	458	305	0.03%	0.004%
54	9.519	2633	2637	2641	rBV4	621	446	0.05%	0.006%
55	9.580	2653	2656	2657	rBV	349	206	0.02%	0.003%
56	9.590	2657	2659	2662	rVB2	428	192	0.02%	0.003%
57	9.609	2662	2665	2668	rBV4	429	300	0.03%	0.004%
58	9.625	2668	2670	2677	rVB4	650	768	0.09%	0.011%
59	9.664	2677	2682	2683	rBV3	731	571	0.06%	0.008%
60	9.712	2694	2697	2700	rBV3	497	367	0.04%	0.005%
61	9.812	2725	2728	2729	rBV2	490	326	0.04%	0.005%
62	9.837	2734	2736	2741	rVB2	477	319	0.04%	0.005%
63	9.870	2743	2746	2748	rBV	385	277	0.03%	0.004%
64	9.921	2759	2762	2766	rBV4	421	366	0.04%	0.005%
65	9.998	2784	2786	2790	rVB3	605	336	0.04%	0.005%
66	10.059	2803	2805	2809	rVB2	509	194	0.02%	0.003%
67	10.098	2814	2817	2818	rBV3	428	225	0.03%	0.003%
68	10.156	2823	2835	2854	rBV	254057	402742	45.50%	5.782%
69	10.294	2873	2878	2880	rBV4	455	421	0.05%	0.006%
70	10.307	2880	2882	2883	rBV	426	196	0.02%	0.003%
71	10.513	2944	2946	2948	rBV2	244	145	0.02%	0.002%
72	10.548	2955	2957	2960	rBV3	390	215	0.02%	0.003%
73	10.644	2985	2987	2990	rBV	207	114	0.01%	0.002%
74	10.670	2990	2995	2996	rBV3	470	303	0.03%	0.004%
75	10.776	3026	3028	3031	rVB3	471	179	0.02%	0.003%
76	10.889	3061	3063	3064	rBV	430	171	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031935.D
 Acq On : 25 Aug 2023 15:30
 Operator : SY/MD
 Sample : 04175-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.188	3144	3156	3179	rBV	520328	814029	91.96%	11.686%
78	11.352	3205	3207	3213	rVB5	874	475	0.05%	0.007%
79	11.564	3262	3273	3293	rBV	432309	672248	75.94%	9.651%
80	11.966	3396	3398	3404	rVB6	460	394	0.04%	0.006%
81	12.091	3434	3437	3442	rBV5	446	436	0.05%	0.006%
82	12.127	3447	3448	3449	rBV	379	116	0.01%	0.002%
83	12.297	3496	3501	3511	rVB7	4703	6888	0.78%	0.099%
84	12.651	3609	3611	3614	rVB2	509	280	0.03%	0.004%
85	12.667	3614	3616	3620	rBV2	524	381	0.04%	0.005%
86	12.747	3638	3641	3644	rBV2	495	422	0.05%	0.006%
87	12.805	3656	3659	3661	rBV3	389	252	0.03%	0.004%
88	12.959	3705	3707	3709	rBV2	405	233	0.03%	0.003%
89	13.078	3742	3744	3749	rVB2	422	295	0.03%	0.004%
90	13.101	3749	3751	3753	rBV3	445	245	0.03%	0.004%
91	13.207	3782	3784	3786	rVB2	749	241	0.03%	0.003%
92	13.358	3827	3831	3832	rBV2	525	385	0.04%	0.006%
93	13.522	3880	3882	3883	rBV2	531	242	0.03%	0.003%
94	13.558	3891	3893	3895	rBV2	345	162	0.02%	0.002%
95	13.725	3940	3945	3947	rBV2	486	462	0.05%	0.007%
96	13.831	3972	3978	3982	rBV5	540	646	0.07%	0.009%
97	13.885	3990	3995	3996	rBV3	504	403	0.05%	0.006%
98	13.937	4009	4011	4012	rBV3	632	256	0.03%	0.004%
99	14.088	4054	4058	4061	rBV4	503	462	0.05%	0.007%
100	14.905	4310	4312	4317	rBV5	814	691	0.08%	0.010%




Sum of corrected areas: 6965873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031935.D
Acq On : 25 Aug 2023 15:30
Operator : SY/MD
Sample : 04175-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

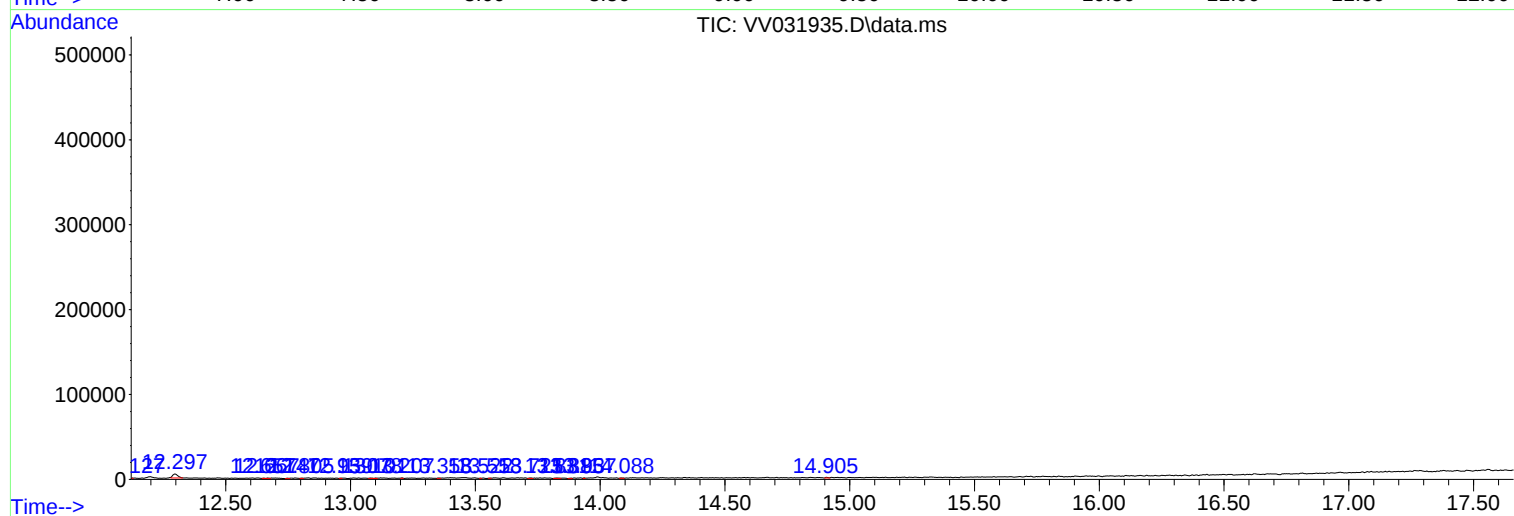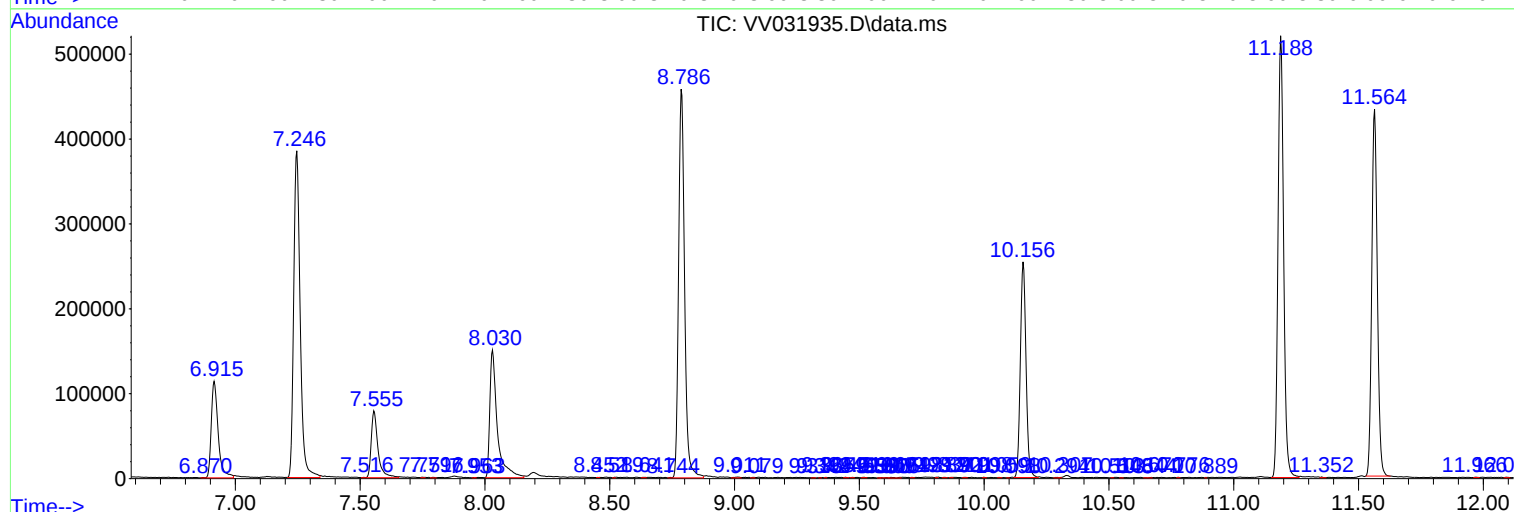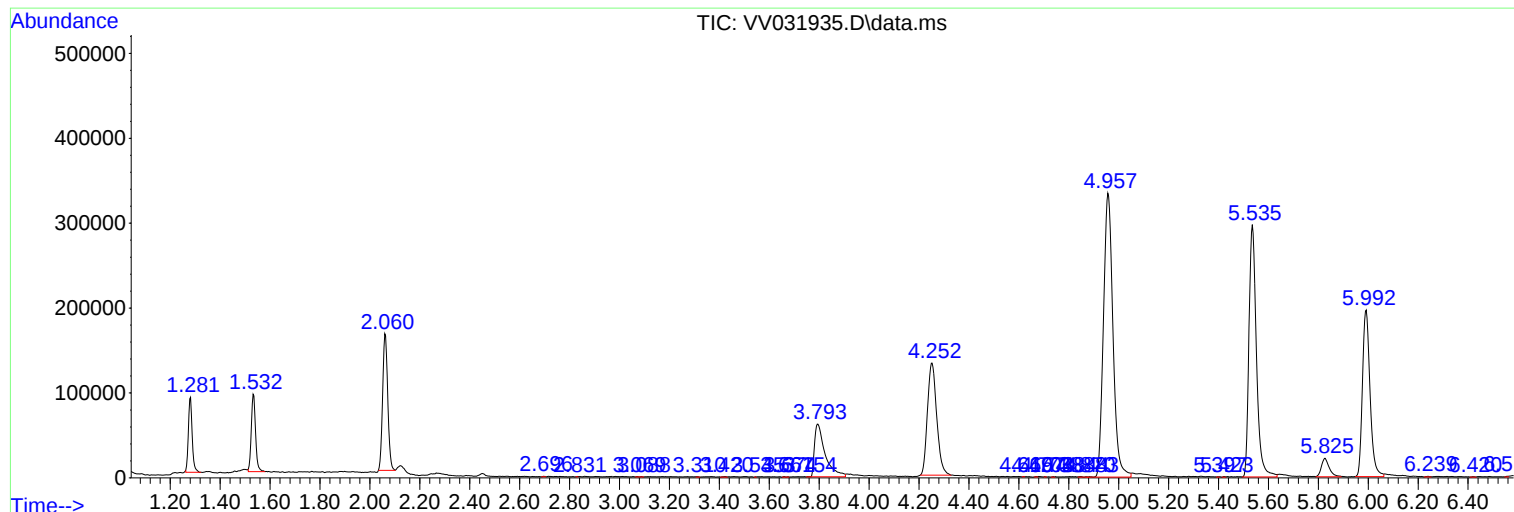

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031935.D
Acq On : 25 Aug 2023 15:30
Operator : SY/MD
Sample : 04175-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031935.D
Acq On : 25 Aug 2023 15:30
Operator : SY/MD
Sample : 04175-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZY9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc