

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031936.D
 Acq On : 25 Aug 2023 15:52
 Operator : SY/MD
 Sample : 04175-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	56	rBV3	2533	1819	0.22%	0.027%
2	1.282	68	75	89	rBV	86050	90989	10.76%	1.345%
3	1.532	146	153	163	rBV	82808	97277	11.50%	1.437%
4	2.063	308	318	330	rBV	152166	224506	26.54%	3.317%
5	2.236	366	372	384	rVB	6653	11828	1.40%	0.175%
6	2.445	431	437	438	rBV5	2720	2077	0.25%	0.031%
7	2.539	464	466	471	rBV4	387	349	0.04%	0.005%
8	2.699	513	516	517	rBV2	862	573	0.07%	0.008%
9	2.973	599	601	606	rVB4	576	448	0.05%	0.007%
10	3.121	644	647	651	rBV3	546	397	0.05%	0.006%
11	3.391	727	731	736	rBV5	630	696	0.08%	0.010%
12	3.449	744	749	752	rBV3	354	397	0.05%	0.006%
13	3.622	799	803	806	rVV3	373	352	0.04%	0.005%
14	3.793	847	856	891	rBV	64478	182715	21.60%	2.700%
15	4.256	983	1000	1024	rBV	126525	334508	39.54%	4.943%
16	4.526	1080	1084	1087	rBV5	507	405	0.05%	0.006%
17	4.960	1202	1219	1246	rBV3	317655	845918	100.00%	12.500%
18	5.191	1289	1291	1294	rVB5	680	402	0.05%	0.006%
19	5.275	1315	1317	1322	rVB4	1128	741	0.09%	0.011%
20	5.301	1322	1325	1328	rBV3	435	340	0.04%	0.005%
21	5.407	1355	1358	1359	rBV2	557	320	0.04%	0.005%
22	5.539	1386	1399	1428	rBV	277895	581447	68.74%	8.592%
23	5.828	1478	1489	1510	rBV2	22099	46974	5.55%	0.694%
24	5.995	1527	1541	1562	rBV	190443	400988	47.40%	5.925%
25	6.182	1597	1599	1603	rVB5	998	652	0.08%	0.010%
26	6.294	1631	1634	1637	rBV2	382	345	0.04%	0.005%
27	6.352	1649	1652	1656	rBV5	674	419	0.05%	0.006%
28	6.391	1660	1664	1668	rBV4	396	406	0.05%	0.006%
29	6.571	1711	1720	1721	rBV4	1324	1579	0.19%	0.023%
30	6.748	1772	1775	1779	rVB4	498	494	0.06%	0.007%
31	6.870	1808	1813	1817	rBV4	365	424	0.05%	0.006%
32	6.918	1817	1828	1857	rBV2	108043	209053	24.71%	3.089%
33	7.246	1919	1930	1961	rBV	364889	661715	78.22%	9.778%
34	7.558	2016	2027	2054	rBV	76208	139833	16.53%	2.066%
35	7.728	2076	2080	2084	rVB5	585	505	0.06%	0.007%
36	7.793	2095	2100	2103	rBV6	706	590	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031936.D
 Acq On : 25 Aug 2023 15:52
 Operator : SY/MD
 Sample : 04175-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.838	2108	2114	2115	rBV3	626	573	0.07%	0.008%
38	7.876	2119	2126	2129	rBV4	1104	1252	0.15%	0.019%
39	8.030	2165	2174	2208	rBV	150272	309417	36.58%	4.572%
40	8.194	2220	2225	2240	rVB5	4935	9402	1.11%	0.139%
41	8.622	2356	2358	2362	rVB3	754	430	0.05%	0.006%
42	8.789	2398	2410	2445	rBV	431202	729179	86.20%	10.775%
43	9.088	2500	2503	2515	rVB7	1276	2199	0.26%	0.032%
44	9.149	2517	2522	2524	rBV3	516	425	0.05%	0.006%
45	9.204	2536	2539	2542	rBV3	581	465	0.05%	0.007%
46	9.239	2542	2550	2554	rVB5	629	826	0.10%	0.012%
47	9.329	2574	2578	2581	rBV2	374	360	0.04%	0.005%
48	9.493	2621	2629	2632	rBV4	1256	1709	0.20%	0.025%
49	9.680	2684	2687	2691	rBV4	387	350	0.04%	0.005%
50	9.866	2741	2745	2746	rBV3	929	654	0.08%	0.010%
51	9.953	2771	2772	2777	rVB2	716	472	0.06%	0.007%
52	9.979	2777	2780	2783	rBV4	501	372	0.04%	0.005%
53	10.156	2821	2835	2853	rBV	248191	395741	46.78%	5.848%
54	10.265	2867	2869	2872	rVB3	728	348	0.04%	0.005%
55	10.326	2881	2888	2890	rBV5	1828	1788	0.21%	0.026%
56	10.403	2907	2912	2913	rBV3	433	344	0.04%	0.005%
57	10.490	2931	2939	2942	rBV4	1022	1513	0.18%	0.022%
58	10.644	2981	2987	2990	rBV4	706	771	0.09%	0.011%
59	10.860	3045	3054	3055	rBV5	1285	1404	0.17%	0.021%
60	11.027	3104	3106	3111	rVB3	532	368	0.04%	0.005%
61	11.188	3144	3156	3177	rBV	497802	781321	92.36%	11.545%
62	11.368	3208	3212	3218	rBV4	568	581	0.07%	0.009%
63	11.490	3245	3250	3251	rBV3	741	608	0.07%	0.009%
64	11.509	3252	3256	3259	rVV4	1702	1821	0.22%	0.027%
65	11.564	3262	3273	3294	rVB	406695	652552	77.14%	9.643%
66	11.767	3334	3336	3341	rVB4	473	406	0.05%	0.006%
67	11.796	3341	3345	3349	rVB4	638	602	0.07%	0.009%
68	11.818	3349	3352	3355	rBV2	568	441	0.05%	0.007%
69	12.095	3435	3438	3441	rBV4	751	481	0.06%	0.007%
70	12.178	3459	3464	3465	rBV3	593	488	0.06%	0.007%
71	12.201	3468	3471	3479	rVB4	1432	1529	0.18%	0.023%
72	12.294	3493	3500	3514	rVV8	4655	8682	1.03%	0.128%
73	12.419	3538	3539	3543	rVB	728	355	0.04%	0.005%
74	12.535	3573	3575	3580	rBV3	343	363	0.04%	0.005%
75	12.590	3589	3592	3600	rVB5	971	1058	0.13%	0.016%
76	12.696	3623	3625	3632	rBV4	643	637	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
 Data File : VV031936.D
 Acq On : 25 Aug 2023 15:52
 Operator : SY/MD
 Sample : 04175-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	12.796	3651	3656	3659	rVB4	658	573	0.07%	0.008%
78	12.812	3659	3661	3664	rBV2	446	360	0.04%	0.005%
79	12.831	3665	3667	3672	rVB3	668	504	0.06%	0.007%
80	13.088	3745	3747	3750	rVV2	537	324	0.04%	0.005%
81	13.165	3766	3771	3773	rBV3	637	545	0.06%	0.008%
82	13.246	3792	3796	3801	rBV3	474	578	0.07%	0.009%
83	13.284	3804	3808	3811	rBV5	595	487	0.06%	0.007%
84	13.455	3858	3861	3867	rVB3	1072	906	0.11%	0.013%
85	13.561	3892	3894	3897	rBV2	616	324	0.04%	0.005%
86	13.686	3929	3933	3940	rVV7	1078	1504	0.18%	0.022%
87	13.722	3940	3944	3947	rBV4	398	349	0.04%	0.005%
88	13.750	3951	3953	3956	rBV3	638	371	0.04%	0.005%
89	13.824	3971	3976	3977	rBV4	631	489	0.06%	0.007%
90	13.937	4008	4011	4014	rVB3	633	350	0.04%	0.005%
91	14.252	4108	4109	4113	rVB2	646	348	0.04%	0.005%
92	14.336	4133	4135	4140	rBV5	725	746	0.09%	0.011%
93	14.439	4165	4167	4172	rVB5	469	334	0.04%	0.005%
94	14.599	4213	4217	4219	rBV5	523	401	0.05%	0.006%
95	14.998	4338	4341	4343	rBV3	904	574	0.07%	0.008%
96	15.133	4381	4383	4388	rVB5	772	591	0.07%	0.009%
97	15.156	4388	4390	4394	rBV2	573	590	0.07%	0.009%
98	15.213	4405	4408	4410	rBV4	716	538	0.06%	0.008%
99	15.448	4478	4481	4484	rBV5	699	432	0.05%	0.006%
100	15.509	4498	4500	4503	rVB4	790	361	0.04%	0.005%




Sum of corrected areas: 6767347

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031936.D
Acq On : 25 Aug 2023 15:52
Operator : SY/MD
Sample : 04175-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

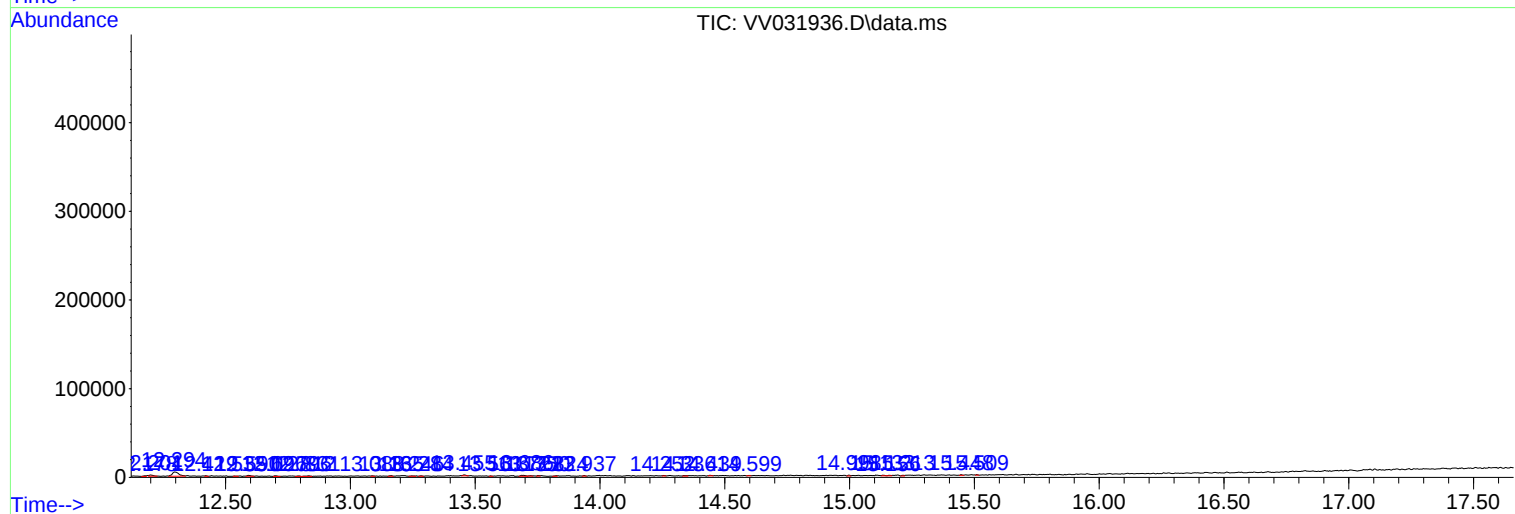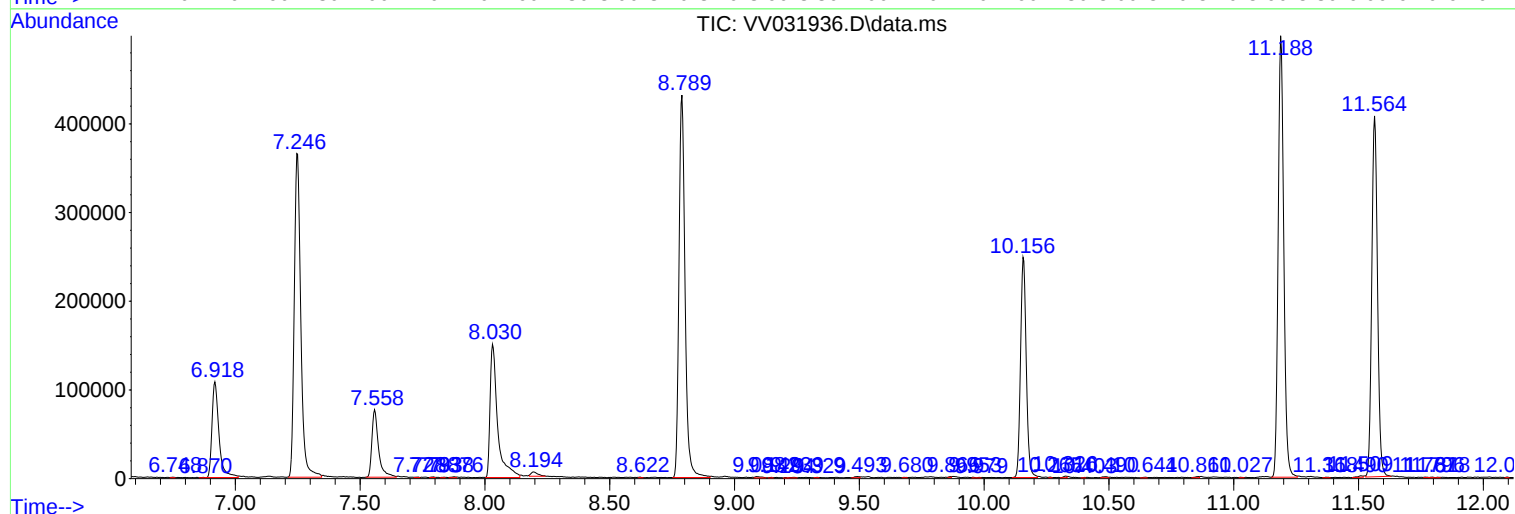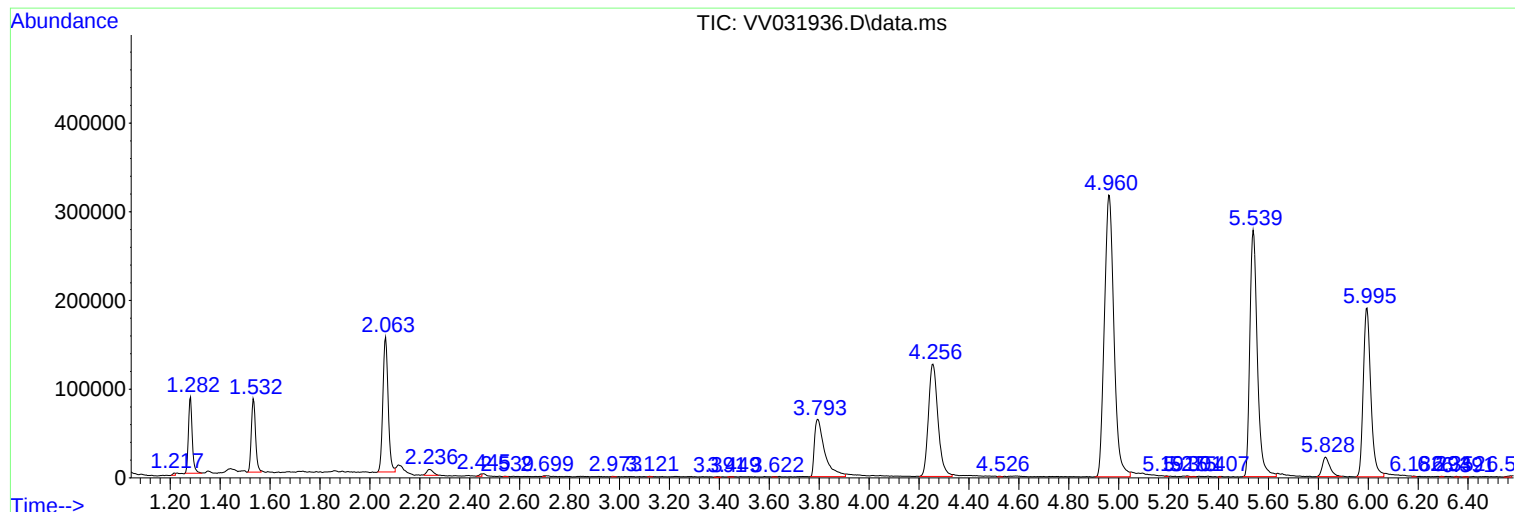

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031936.D
Acq On : 25 Aug 2023 15:52
Operator : SY/MD
Sample : 04175-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082523\
Data File : VV031936.D
Acq On : 25 Aug 2023 15:52
Operator : SY/MD
Sample : 04175-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc