
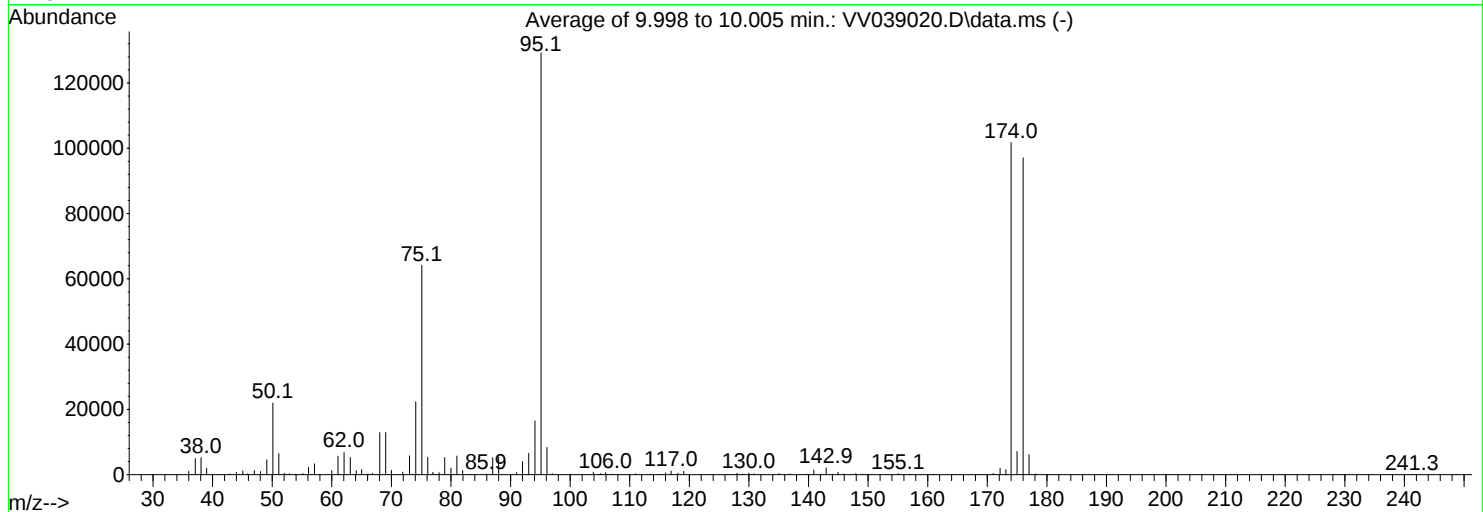


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV082525\
Data File : VV039020.D
Acq On : 25 Aug 2025 08:35
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V082525W.M
Title : SW846 8260
Last Update : Tue Aug 26 02:37:06 2025

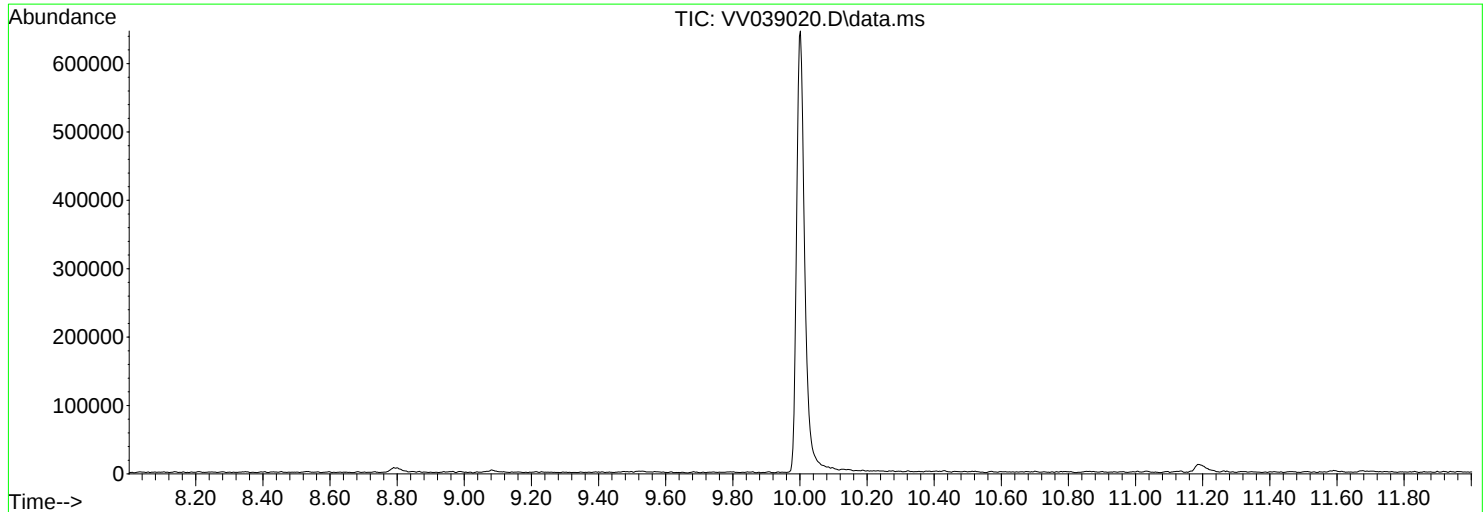

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	21893	PASS
75	95	30	60	49.6	64096	PASS
95	95	100	100	100.0	129224	PASS
96	95	5	9	6.4	8314	PASS
173	174	0.00	2	1.5	1487	PASS
174	95	50	100	78.7	101717	PASS
175	174	5	9	7.0	7115	PASS
176	174	95	101	95.4	97035	PASS
177	176	5	9	6.3	6113	PASS