

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082619\
 Data File : VV012409.D
 Acq On : 26 Aug 2019 18:38
 Operator : SY/MD
 Sample : K4501-10
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GANM5

Quant Time: Aug 27 04:14:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Aug 27 02:19:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	225785	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	220494	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	88687	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48330	4.28	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.60%
7) Chloroethane-d5	1.58	69	34270	4.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.40%
11) 1,1-Dichloroethene-d2	2.13	63	62878	3.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.80%
20) 2-Butanone-d5	3.97	46	151585	49.85	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.70%
24) Chloroform-d	4.40	84	116123	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.08	65	60294	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.10	84	236437	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
36) 1,2-Dichloropropane-d6	6.12	67	74071	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.36	98	187504	3.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.00%
43) trans-1,3-Dichloropropene-	7.66	79	23522	3.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.40%
46) 2-Hexanone-d5	8.14	63	70654	36.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.88%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	43993	4.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	67422	4.57	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.40%


Target Compounds					Ovalue
47) Tetrachloroethene	8.02	164	6865	0.561 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082619\
Data File : VV012409.D
Acq On : 26 Aug 2019 18:38
Operator : SY/MD
Sample : K4501-10
Misc : 25mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GANM5

Quant Time: Aug 27 04:14:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 27 02:19:39 2019
Response via : Initial Calibration

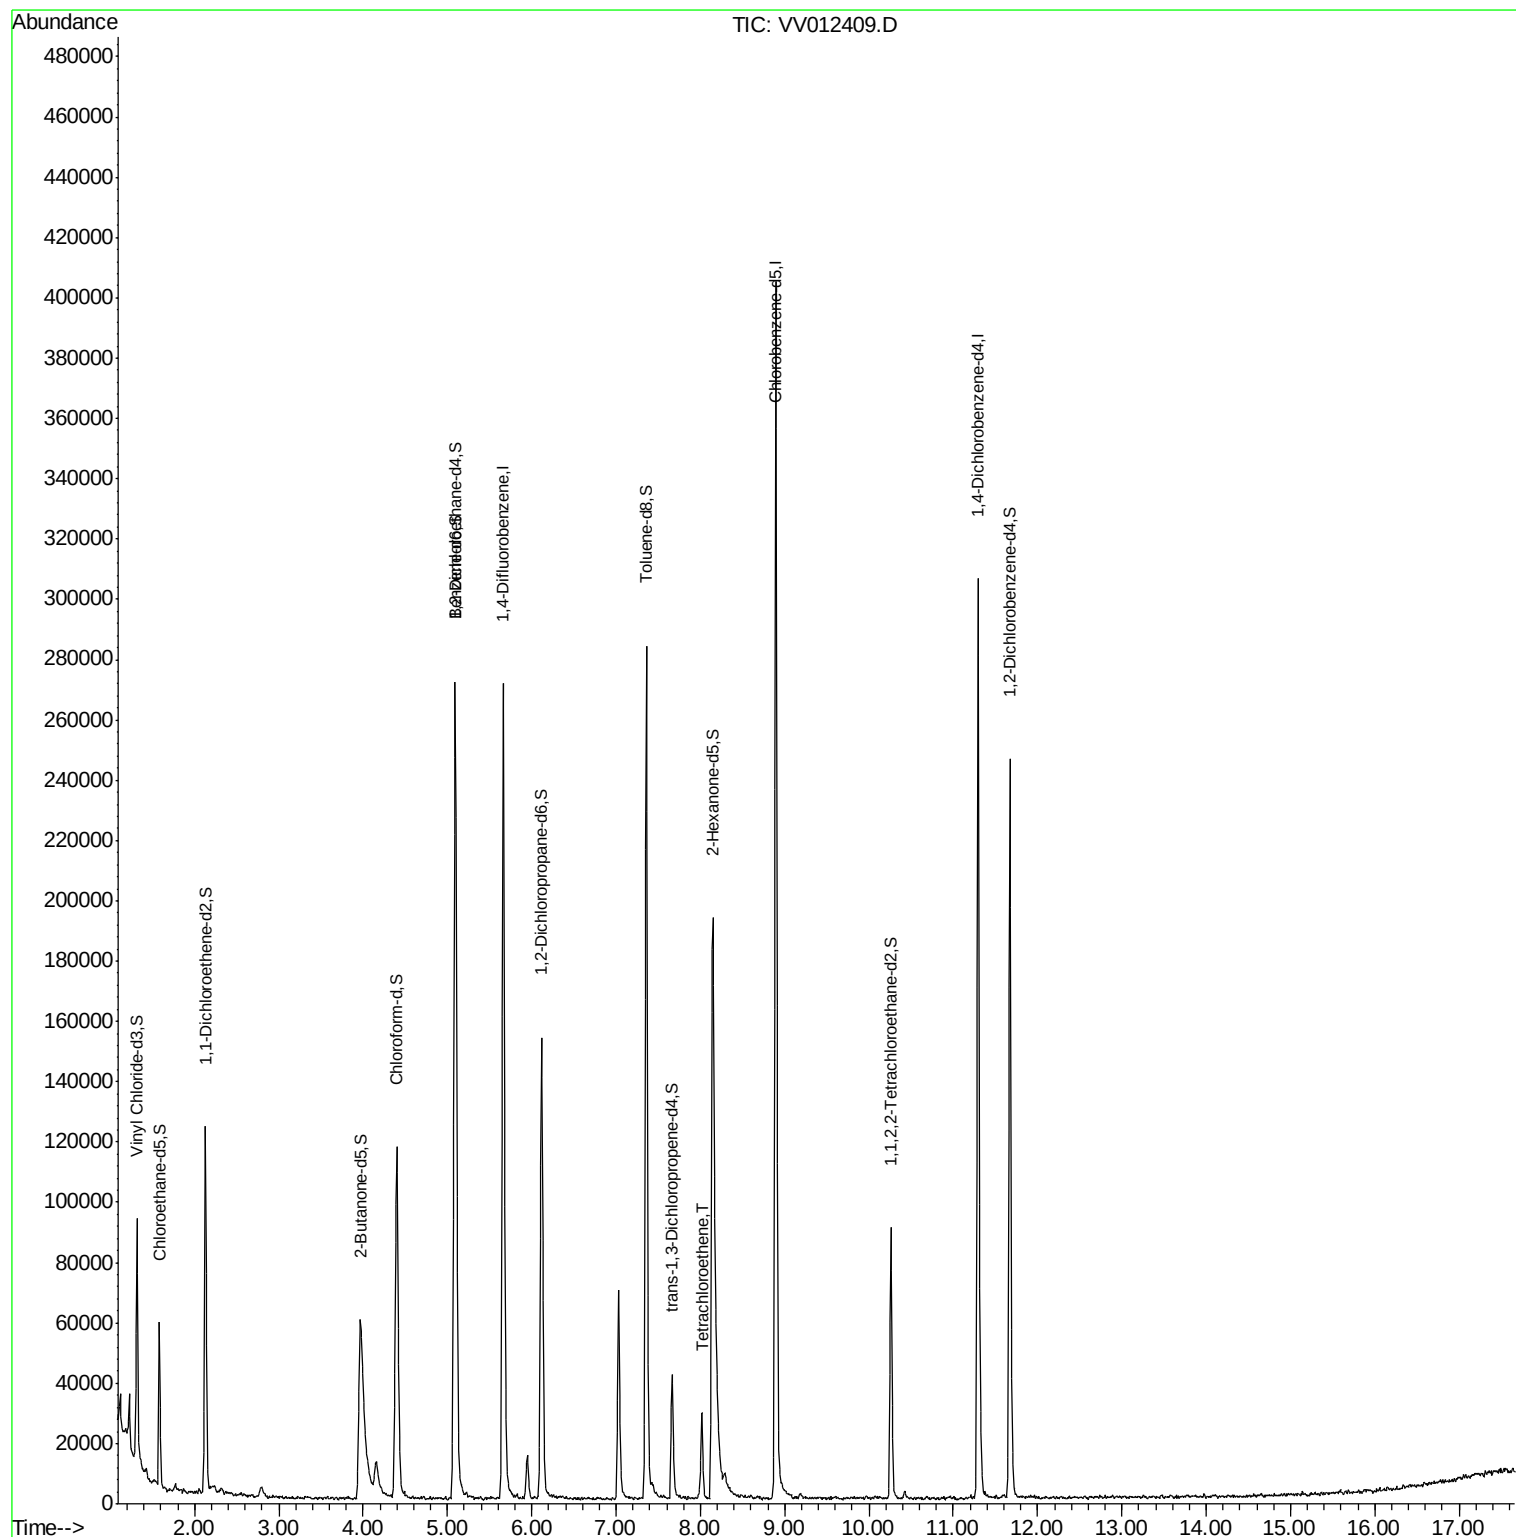

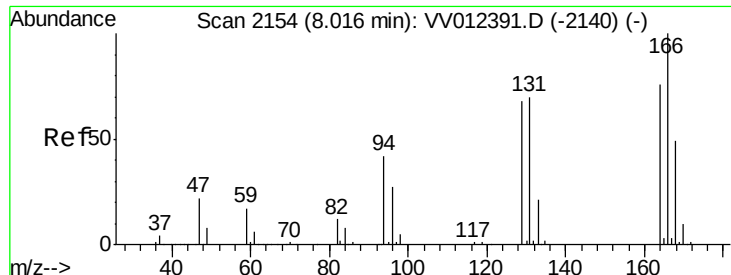

#47

Tetrachloroethene

Concen: 0.561 ug/L

RT: 8.02 min Scan# 2154

Delta R.T. -0.00 min

Lab File: VV012409.D


Acq: 26 Aug 2019 18:38

Instrument :

MSVOA_V

ClientSampleId :

GANM5

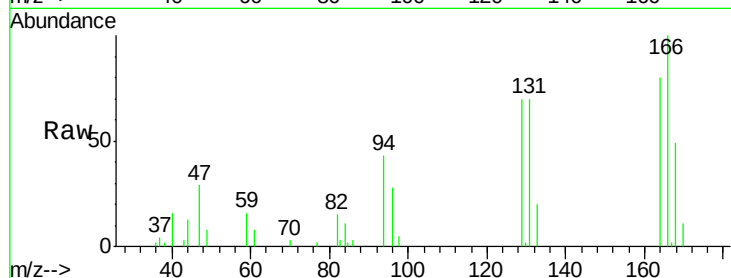

Tot Ion:164 Resp: 6865

Ion Ratio Lower Upper

164 100

129 87.6 60.6 112.6

131 88.5 58.8 109.2

166 125.5 87.6 162.8

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

