


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082619\
Data File : VV012390.D
Acq On : 26 Aug 2019 08:27
Operator : SY/MD
Sample : BFB53
Misc : 5mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB53

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 27 11:12:30 2019

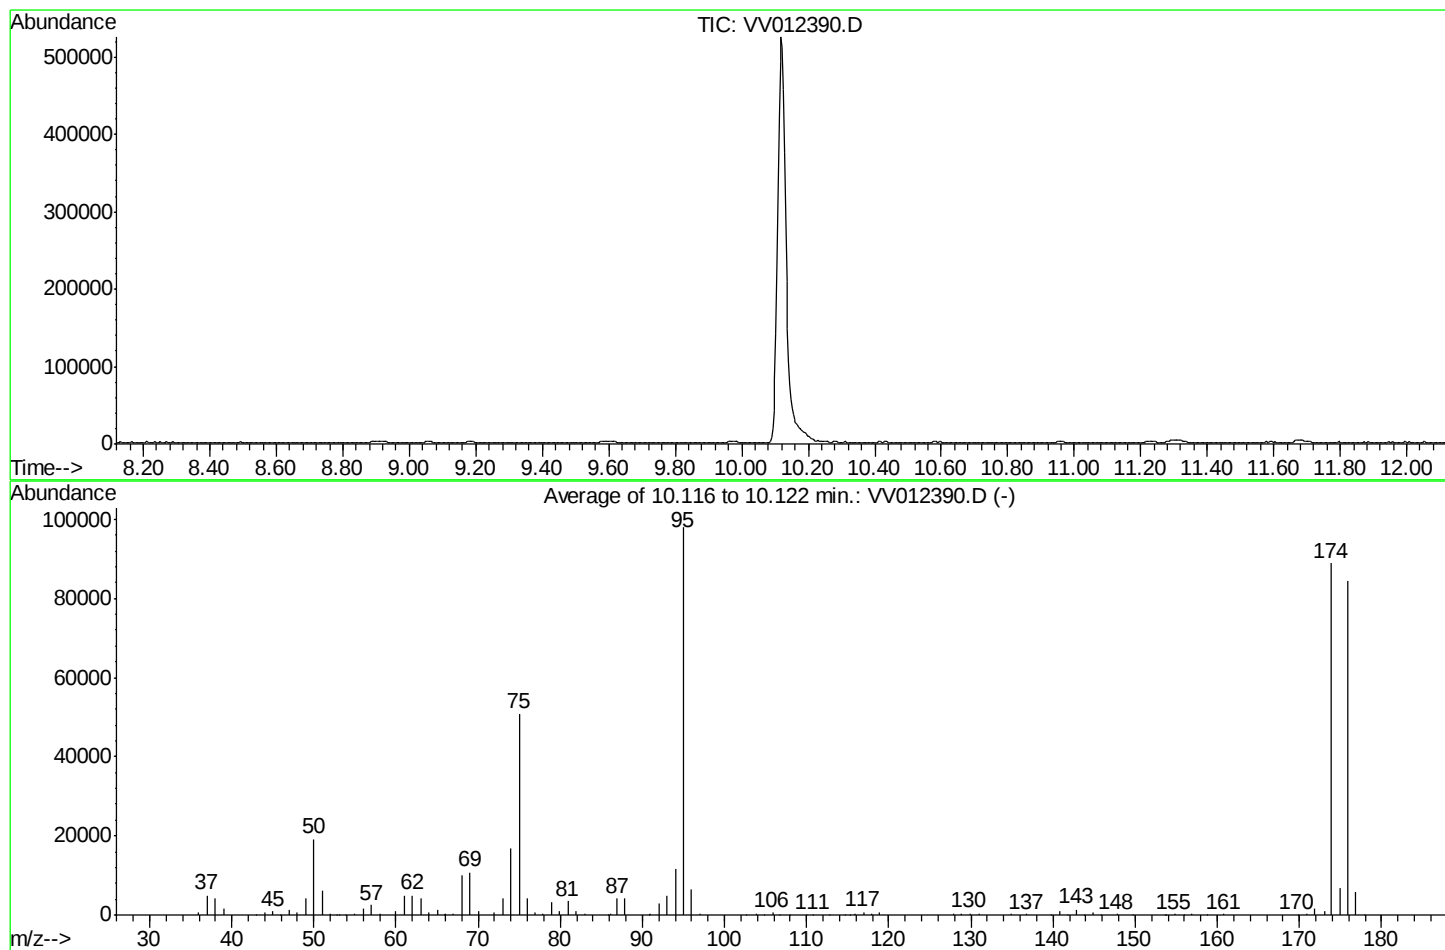

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	19237	PASS
75	95	30	80	51.8	50786	PASS
95	95	100	100	100.0	97962	PASS
96	95	5	9	6.7	6588	PASS
173	174	0.00	2	1.3	1132	PASS
174	95	50	120	90.7	88885	PASS
175	174	5	9	7.6	6765	PASS
176	174	95	101	95.1	84488	PASS
177	176	5	9	6.8	5730	PASS

m/z	Abundance
36.00	951.0
37.00	4966.0
38.00	3920.0
39.00	1831.0
39.90	765.0
42.80	177.0
44.00	1273.0
45.00	1015.0
46.00	286.0
47.00	1207.0
47.90	589.0
49.00	4070.0
50.00	18680.0
51.00	6352.0
52.00	298.0
52.80	147.0
55.00	243.0
56.00	1484.0
57.00	2400.0
58.00	231.0
59.90	855.0
61.00	4543.0
62.00	4904.0
63.00	4280.0
64.00	840.0
65.00	1357.0
65.90	167.0
66.10	175.0
67.00	322.0
68.00	9621.0
69.00	10432.0
70.00	927.0
72.00	650.0
73.00	4075.0
74.00	16752.0
75.00	50144.0
76.00	4259.0
76.90	567.0
77.90	442.0
78.90	3315.0
79.90	1014.0
80.90	3337.0
81.90	955.0
83.00	186.0
86.20	239.0
86.90	4071.0
87.90	3927.0
90.80	368.0
92.00	2875.0
93.00	4678.0
94.00	11358.0
95.00	94904.0
96.00	6447.0
97.20	200.0
102.60	131.0
103.90	490.0
104.80	158.0
105.80	553.0
107.90	110.0
109.90	111.0
110.80	157.0
112.70	101.0
115.80	335.0
116.90	669.0
117.80	331.0
118.90	684.0
127.90	406.0
128.80	232.0
129.90	441.0
131.00	139.0
134.90	153.0
136.80	251.0
139.70	124.0
140.90	895.0
142.90	1319.0
143.80	162.0
144.80	556.0
145.70	186.0
147.80	196.0
149.70	115.0
153.60	110.0
154.90	336.0
156.00	121.0
156.80	178.0
158.80	138.0
160.80	222.0
171.00	244.0
171.80	1437.0
173.10	1634.0
173.90	85432.0
174.90	6636.0
175.90	79600.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

176.90	5588.0
177.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
36.00	879.0
37.00	5213.0
38.00	4309.0
39.10	1873.0
39.90	750.0
42.90	163.0
44.00	1322.0
45.00	976.0
45.90	301.0
47.10	1313.0
48.00	605.0
49.00	4303.0
50.00	19784.0
51.00	6270.0
52.00	328.0
53.10	180.0
55.00	321.0
56.00	1617.0
57.00	2659.0
58.00	243.0
59.90	914.0
61.00	4999.0
62.00	5159.0
63.00	4557.0
63.90	790.0
65.00	1463.0
66.10	193.0
67.00	348.0
68.00	10246.0
69.00	11238.0
70.00	888.0
72.00	693.0
73.00	4417.0
74.00	17336.0
75.00	52528.0
76.00	4331.0
77.00	651.0
77.90	435.0
78.90	3403.0
79.90	1033.0
80.90	3540.0
81.90	1029.0
83.10	187.0
85.80	204.0
86.20	235.0
86.90	4327.0
87.90	4160.0
91.00	384.0
92.00	3119.0
93.00	5179.0
94.00	11945.0
95.00	100632.0
96.00	6764.0
97.10	190.0
102.60	119.0
103.90	512.0
104.80	174.0
105.90	641.0
110.80	168.0
114.70	111.0
115.20	104.0
115.90	366.0
116.90	723.0
117.90	357.0
118.90	721.0
127.90	439.0
128.80	217.0
129.90	433.0
131.00	187.0
134.80	185.0
136.80	342.0
139.70	188.0
140.90	844.0
141.80	119.0
142.90	1442.0
143.90	157.0
144.80	604.0
145.80	159.0
147.80	206.0
149.70	129.0
154.80	320.0
156.00	123.0
156.90	164.0
158.80	142.0
160.80	200.0
170.90	216.0
171.90	1576.0
173.10	1762.0
173.90	91160.0
174.90	6922.0
175.90	86688.0
176.90	5879.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

177.90

155.0

Instrument :

MSVOA_V

ClientSampleId :

BFB53

m/z	Abundance
36.00	805.0
37.00	4711.0
38.00	4364.0
39.10	1736.0
40.00	829.0
43.00	164.0
44.00	1273.0
45.00	893.0
45.90	278.0
47.10	1313.0
48.00	543.0
49.00	3915.0
50.00	19248.0
51.00	5736.0
52.10	340.0
53.10	207.0
53.80	109.0
55.00	346.0
56.00	1579.0
57.00	2844.0
58.00	229.0
60.00	880.0
61.00	4911.0
62.00	4926.0
63.00	4224.0
64.00	711.0
65.00	1405.0
66.00	197.0
66.90	324.0
68.00	10174.0
69.00	10700.0
70.00	777.0
72.00	695.0
73.00	4426.0
74.00	16448.0
75.00	49688.0
76.00	4193.0
77.00	644.0
77.80	396.0
78.90	3342.0
79.90	994.0
80.90	3520.0
81.90	944.0
83.10	153.0
85.70	173.0
86.10	212.0
86.90	4212.0
87.90	4115.0
91.00	381.0
92.00	3012.0
93.00	5036.0
94.00	11674.0
95.00	98352.0
96.00	6553.0
97.00	197.0
103.90	482.0
104.80	181.0
105.90	586.0
106.70	116.0
110.80	135.0
112.80	100.0
114.70	120.0
115.90	424.0
116.90	699.0
117.90	392.0
118.90	688.0
127.80	380.0
128.70	206.0
129.80	399.0
131.00	192.0
134.80	202.0
136.80	371.0
139.70	183.0
140.90	782.0
141.70	122.0
142.90	1372.0
143.90	144.0
144.90	603.0
145.90	142.0
147.80	213.0
149.70	132.0
153.80	101.0
154.80	260.0
155.90	115.0
156.90	175.0
158.80	188.0
160.80	129.0
169.80	102.0
170.80	196.0
171.90	1616.0
173.90	90064.0
174.90	6739.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

175.90	87176.0
176.90	5725.0
177.90	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53

m/z	Abundance
35.80	107.0
39.10	139.0
39.90	835.0
41.20	115.0
43.00	115.0
43.90	507.0
45.80	117.0
57.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB53