

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082620\
 Data File : VV018100.D
 Acq On : 26 Aug 2020 10:17
 Operator : SY/MD
 Sample : VV0826MBL01
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Quant Time: Aug 27 02:07:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 27 02:00:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	266170	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	260603	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	125231	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	98405	48.46	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.92%
7) Chloroethane-d5	1.58	69	85911	51.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.42%
11) 1,1-Dichloroethene-d2	2.12	63	149903	38.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.18%
21) 2-Butanone-d5	3.91	46	117576	88.39	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.39%
24) Chloroform-d	4.37	84	175587	47.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.05	65	121077	50.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.84%
32) Benzene-d6	5.07	84	364310	50.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.44%
36) 1,2-Dichloropropane-d6	6.09	67	117191	49.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.82%
41) Toluene-d8	7.33	98	320951	49.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.38%
43) trans-1,3-Dichloropropene-	7.64	79	53576	50.31	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.62%
47) 2-Hexanone-d5	8.11	63	58496	77.63	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.63%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	137681	45.03	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.06%
64) 1,2-Dichlorobenzene-d4	11.65	152	133015	53.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.94%


Target Compounds					Ovalue
25) Chloroform	4.40	83	8528	2.266 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082620\
Data File : VV018100.D
Acq On : 26 Aug 2020 10:17
Operator : SY/MD
Sample : VV0826MBL01
Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK93

Quant Time: Aug 27 02:07:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 27 02:00:22 2020
Response via : Initial Calibration

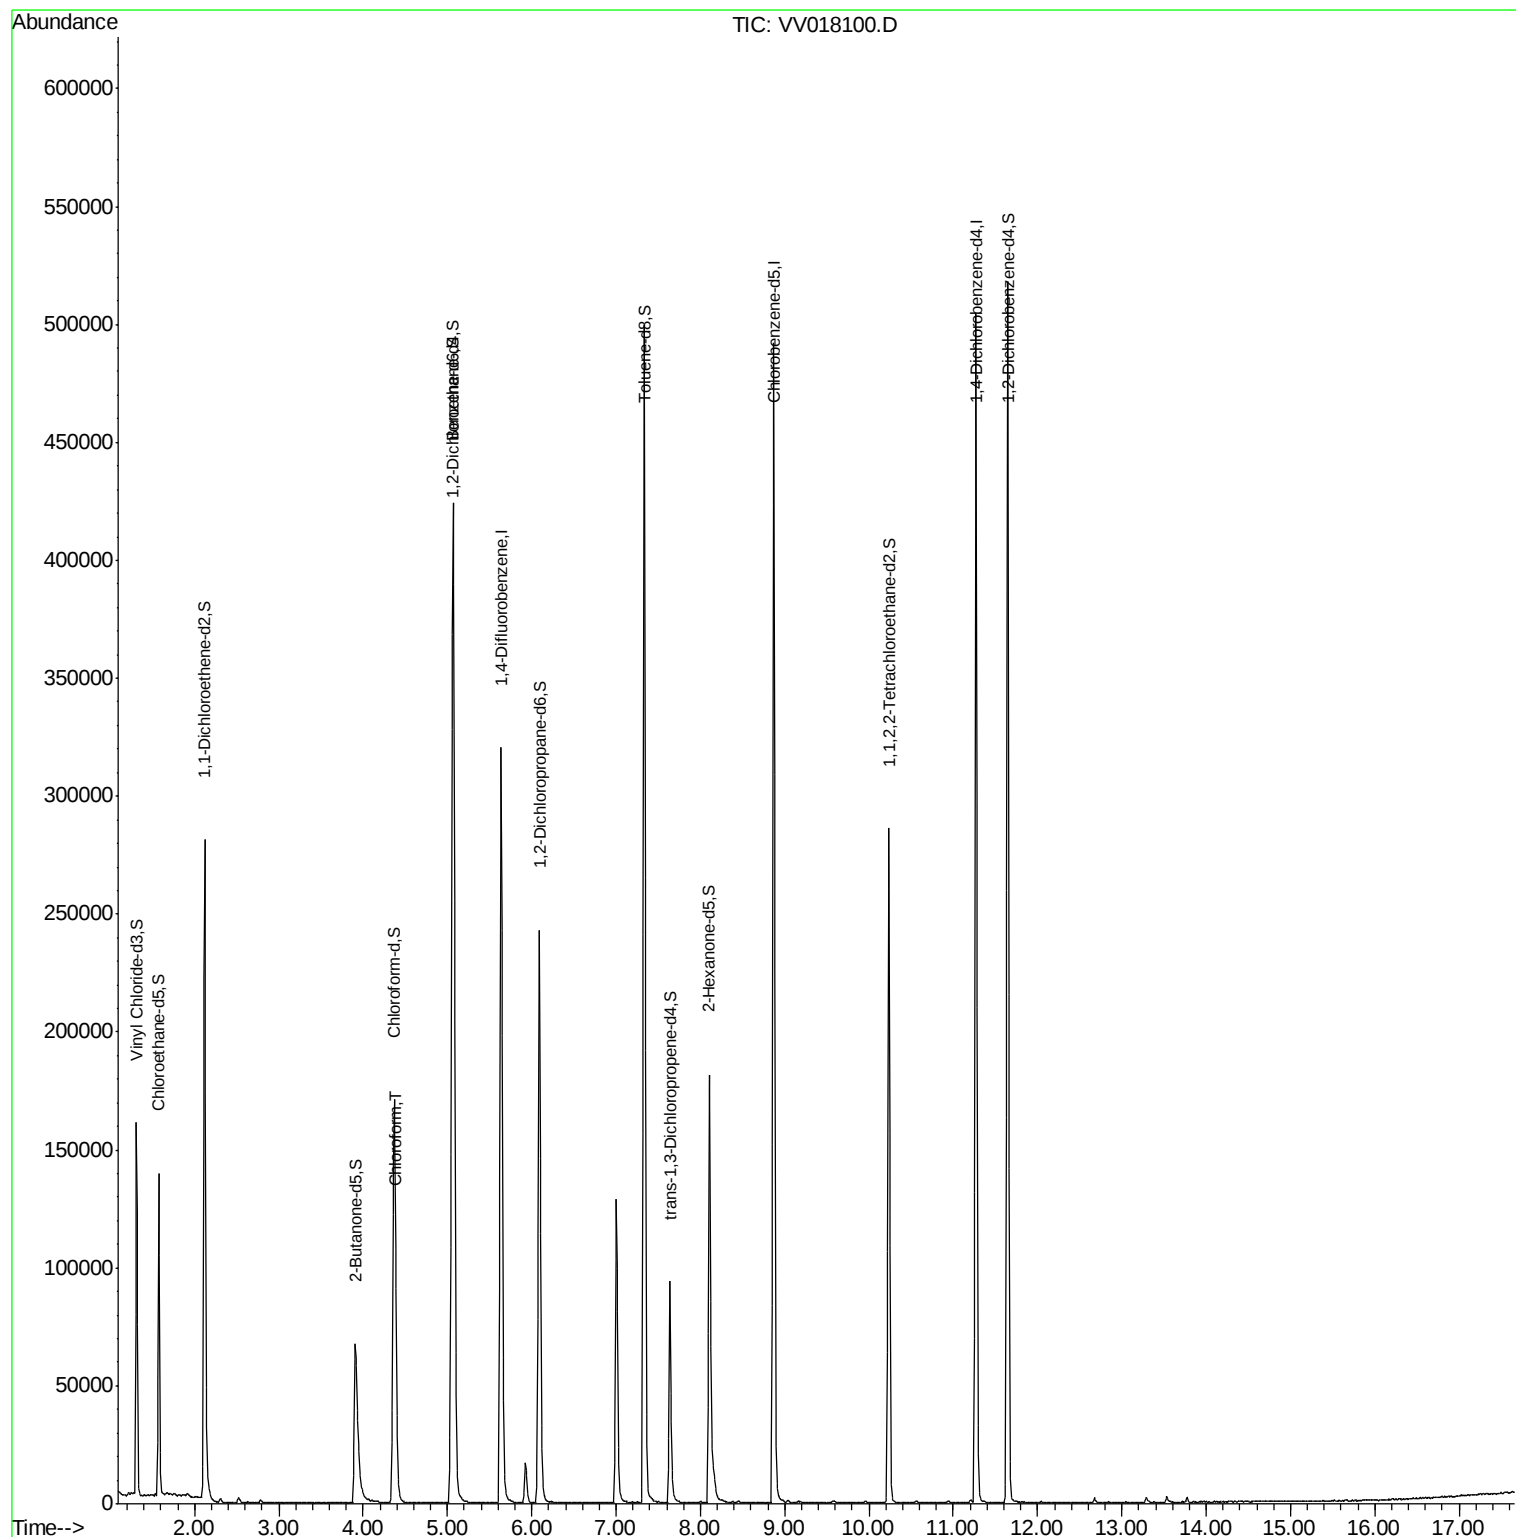

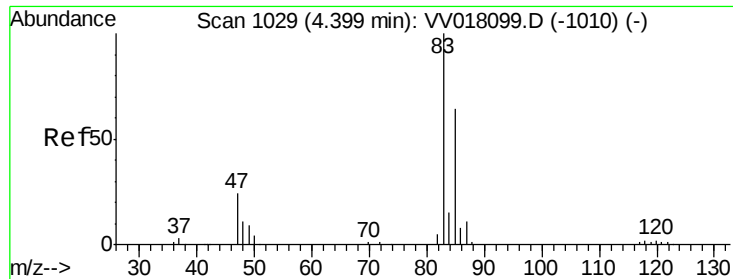

#25
 Chloroform
 Concen: 2.266 ug/L
 RT: 4.40 min Scan# 1028
 Delta R.T. -0.00 min
 Lab File: VV018100.D
 Acq: 26 Aug 2020 10:17

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK93

Tot Ion: 83 Resp: 8528
 Ion Ratio Lower Upper
 83 100
 85 69.1 45.5 84.5

