


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082620\
 Data File : VV018098.D
 Acq On : 26 Aug 2020 08:49
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Thu Aug 27 02:00:22 2020

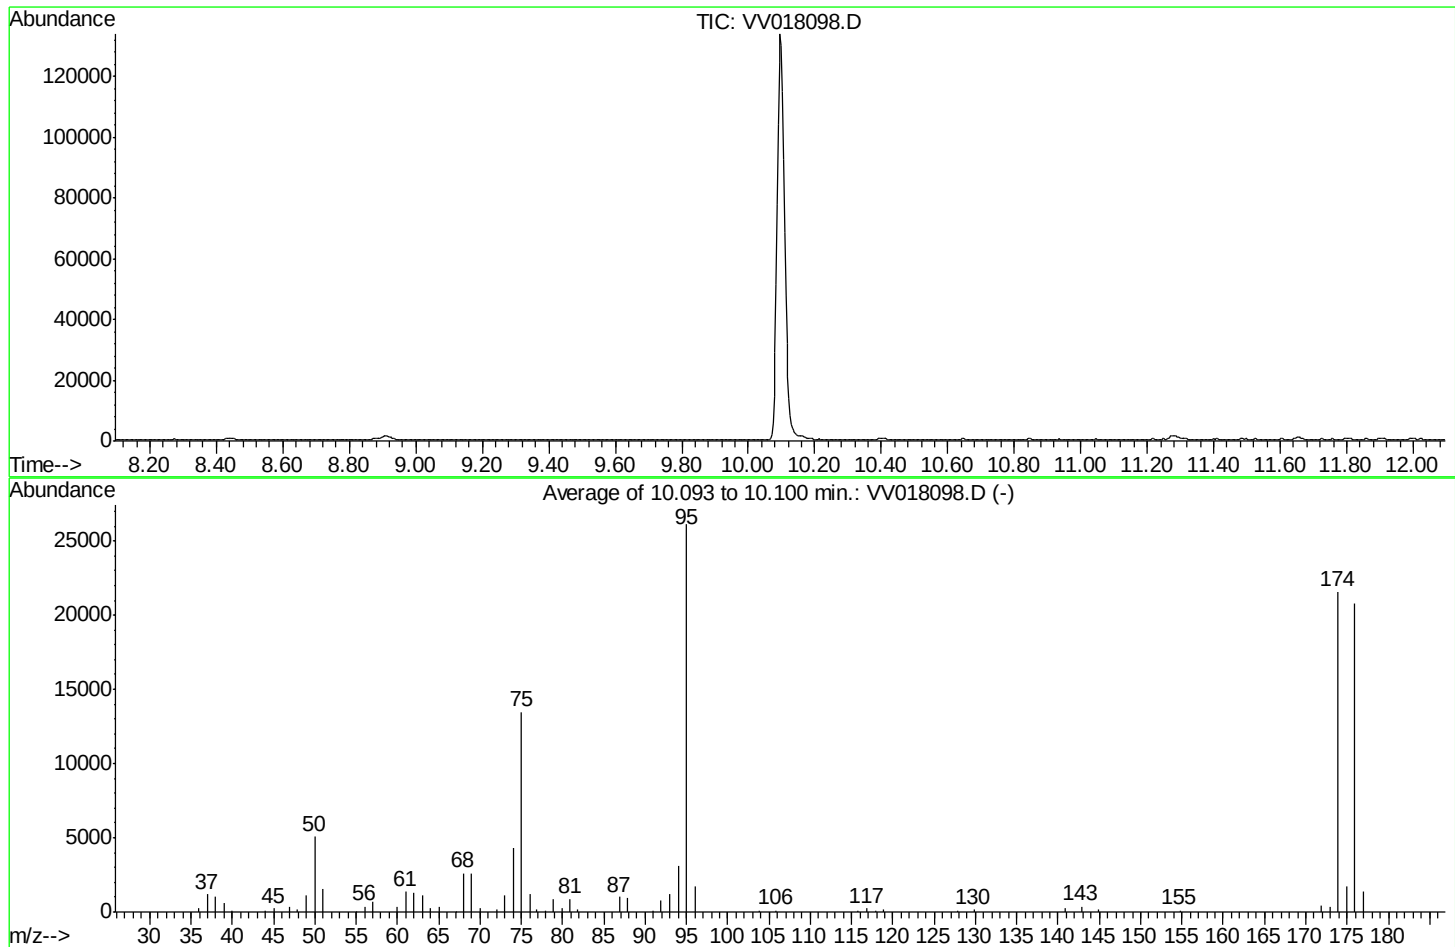

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	5058	PASS
75	95	30	80	51.6	13471	PASS
95	95	100	100	100.0	26117	PASS
96	95	5	9	6.7	1751	PASS
173	174	0.00	2	1.5	331	PASS
174	95	50	120	82.7	21586	PASS
175	174	5	9	7.8	1690	PASS
176	174	95	101	96.4	20800	PASS
177	176	5	9	6.5	1356	PASS

m/z	Abundance
35.00	219.0
37.00	1164.0
38.00	1034.0
39.00	653.0
39.00	252.0
44.00	485.0
45.00	268.0
47.00	387.0
47.00	149.0
49.00	1042.0
50.00	4988.0
51.00	1612.0
56.00	372.0
57.00	674.0
59.00	299.0
61.00	1304.0
62.00	1328.0
63.00	1194.0
64.00	246.0
65.00	361.0
68.00	2630.0
69.00	2476.0
70.00	302.0
72.00	112.0
73.00	1064.0
74.00	4155.0
75.00	13254.0
76.00	1125.0
76.00	199.0
78.00	116.0
78.00	845.0
79.00	297.0
80.00	897.0
81.00	204.0
86.00	941.0
87.00	920.0
91.00	104.0
92.00	801.0
93.00	1111.0
94.00	3054.0
95.00	25096.0
96.00	1749.0
105.00	117.0
115.00	128.0
116.00	162.0
118.00	150.0
129.00	142.0
140.00	223.0
142.00	349.0
144.00	171.0
154.00	118.0
171.00	432.0
172.00	310.0
173.00	20296.0
174.00	1679.0
175.00	19640.0
176.00	1353.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	265.0
37.00	1221.0
38.00	1068.0
39.00	669.0
39.90	221.0
43.90	445.0
45.00	255.0
46.90	373.0
47.90	156.0
49.00	1127.0
50.00	5245.0
51.00	1602.0
55.00	104.0
56.00	384.0
56.90	696.0
59.90	333.0
61.00	1402.0
62.00	1332.0
63.00	1193.0
64.00	249.0
65.00	391.0
68.00	2701.0
69.00	2670.0
70.00	270.0
72.00	141.0
73.00	1177.0
74.00	4471.0
75.00	13983.0
76.00	1242.0
76.90	193.0
77.90	107.0
78.90	911.0
79.90	316.0
80.90	906.0
81.80	227.0
86.90	1007.0
87.90	1004.0
91.00	136.0
91.90	857.0
93.00	1223.0
94.00	3178.0
95.00	27104.0
96.00	1804.0
103.70	123.0
105.90	126.0
115.80	138.0
116.90	177.0
117.90	118.0
118.80	161.0
127.80	112.0
129.90	151.0
140.80	249.0
142.80	379.0
144.90	166.0
154.70	124.0
171.90	473.0
172.90	336.0
173.90	22160.0
174.90	1740.0
175.90	21496.0
176.90	1377.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

m/z	Abundance
35.90	291.0
37.00	1162.0
38.00	1055.0
39.00	585.0
39.90	200.0
43.90	445.0
45.00	219.0
46.90	353.0
47.90	160.0
49.00	1138.0
50.00	4943.0
51.00	1437.0
56.00	342.0
56.90	696.0
59.90	337.0
61.00	1381.0
62.00	1214.0
63.00	1108.0
64.00	239.0
65.00	374.0
67.10	103.0
68.00	2511.0
69.00	2561.0
70.00	214.0
72.00	167.0
73.00	1156.0
74.00	4371.0
75.00	13177.0
76.00	1170.0
76.90	173.0
78.90	900.0
79.90	283.0
80.90	914.0
81.90	216.0
86.90	1047.0
87.90	993.0
91.00	151.0
91.90	780.0
93.00	1215.0
94.00	2991.0
95.00	26152.0
96.00	1700.0
103.80	135.0
105.80	126.0
115.80	111.0
116.80	173.0
117.00	173.0
117.90	125.0
118.80	160.0
127.80	103.0
129.80	134.0
140.80	252.0
142.80	360.0
145.00	149.0
154.70	107.0
171.90	483.0
172.90	349.0
173.90	22304.0
175.00	1652.0
175.90	21264.0
176.90	1340.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82

Scan 2790 (10.061 min): VV018098.D
BFB82

m/z	Abundance
39.90	139.0
44.00	362.0

Instrument :
MSVOA_V
ClientSampleId :
BFB82