

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082621\
 Data File : VV021956.D
 Acq On : 26 Aug 2021 10:35
 Operator : SY/MD
 Sample : VV0826MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Quant Time: Aug 27 03:47:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 27 03:46:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	398694	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	382186	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	196727	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	103037	33.058	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	66.120%
7) Chloroethane-d5	1.564	69	91443	38.878	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	77.760%
11) 1,1-Dichloroethene-d2	2.104	63	142009	28.623	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.240%#
21) 2-Butanone-d5	3.876	46	196123	101.173	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.170%
24) Chloroform-d	4.352	84	223103	41.315	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.620%
26) 1,2-Dichloroethane-d4	5.034	65	148427	47.784	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.560%
32) Benzene-d6	5.053	84	488068	44.409	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.820%
36) 1,2-Dichloropropane-d6	6.072	67	156766	45.805	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.600%
41) Toluene-d8	7.320	98	459091	45.194	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.380%
43) trans-1,3-Dichloroprop...	7.625	79	73547	43.665	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.320%
47) 2-Hexanone-d5	8.088	63	117348	104.614	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.610%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	193839	45.704	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	194704	47.823	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.640%
Target Compounds						
					Qvalue	
25) Chloroform	4.381	83	12067	2.278	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082621\
Data File : VV021956.D
Acq On : 26 Aug 2021 10:35
Operator : SY/MD
Sample : VV0826MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Time: Aug 27 03:47:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 27 03:46:52 2021
Response via : Initial Calibration

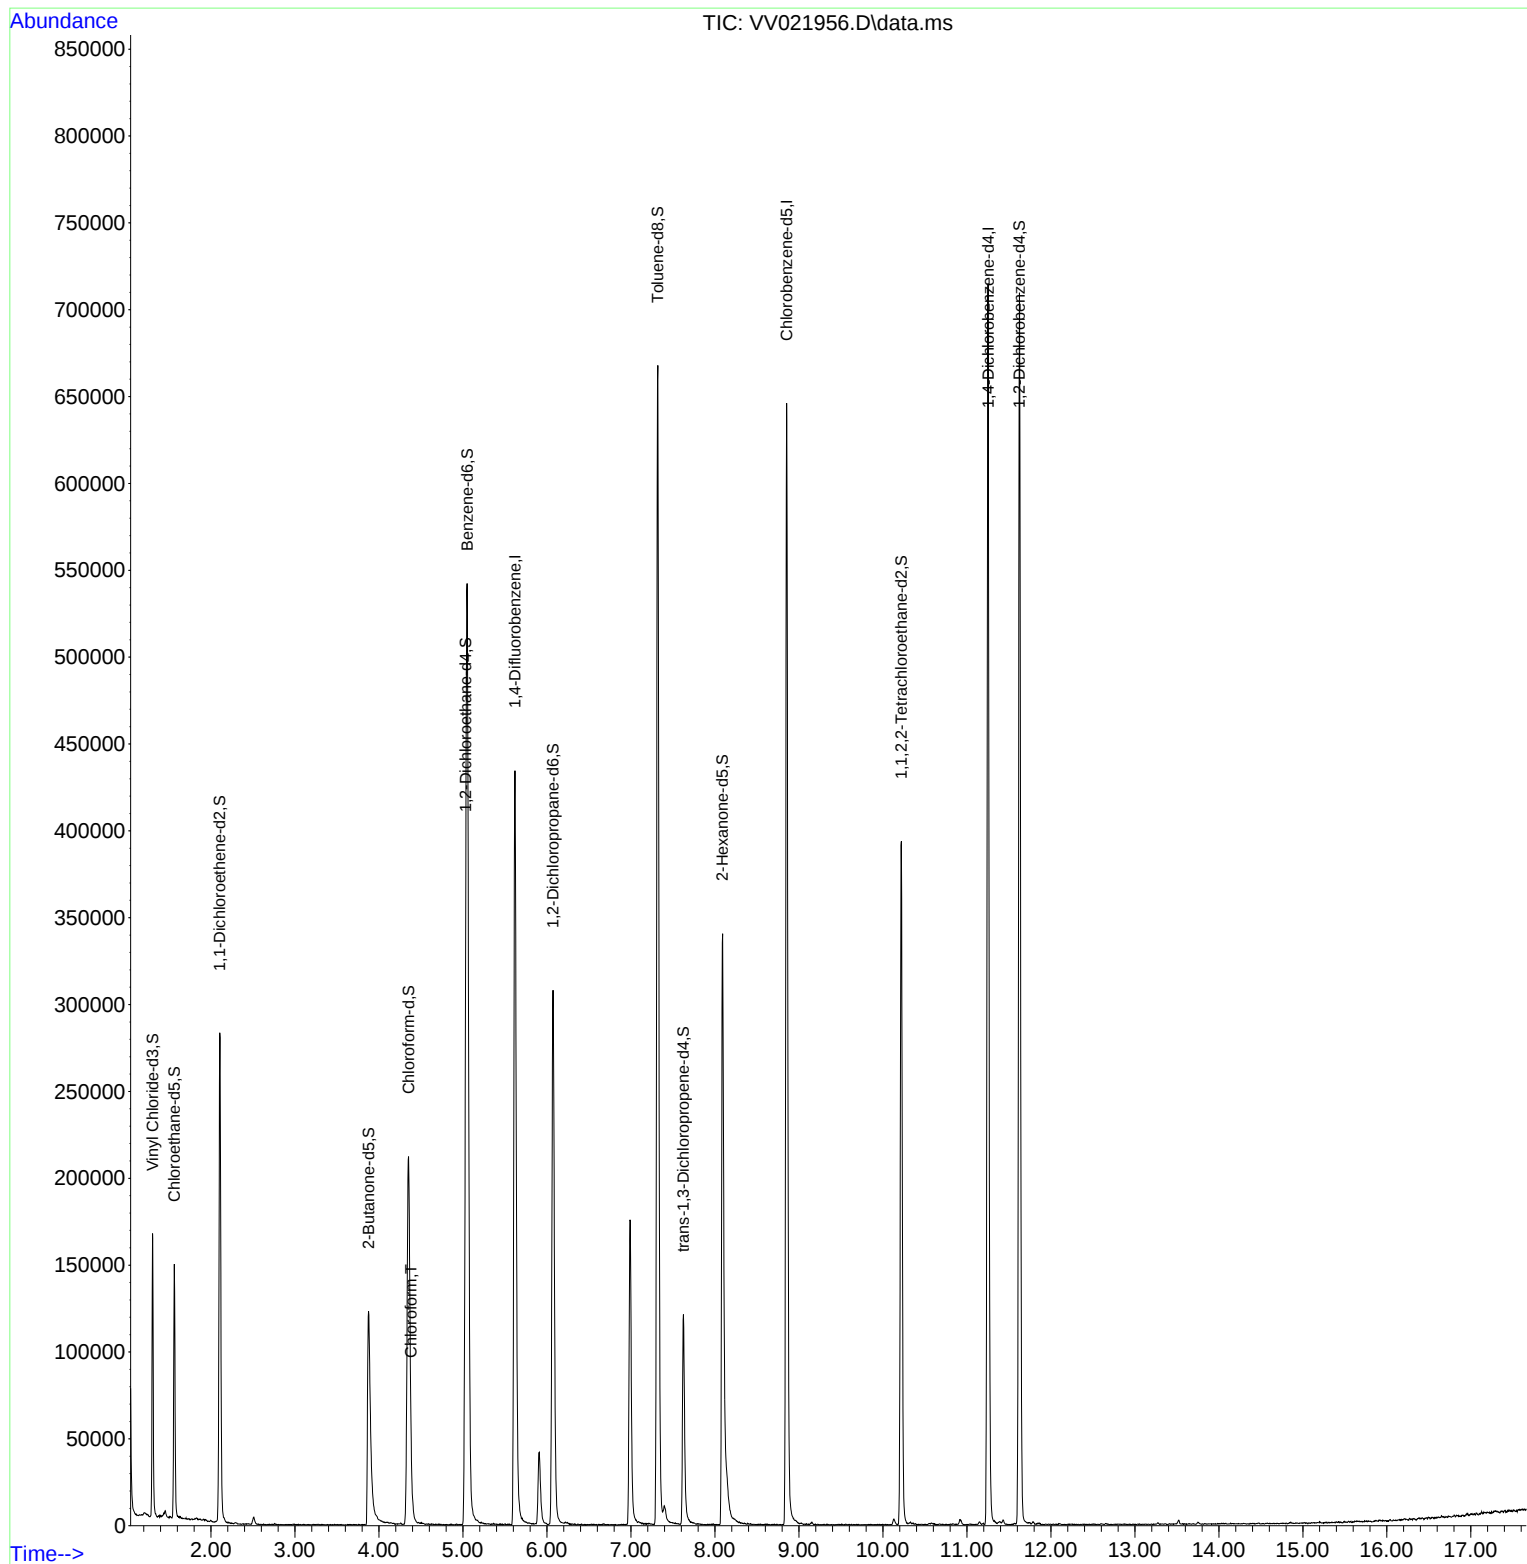

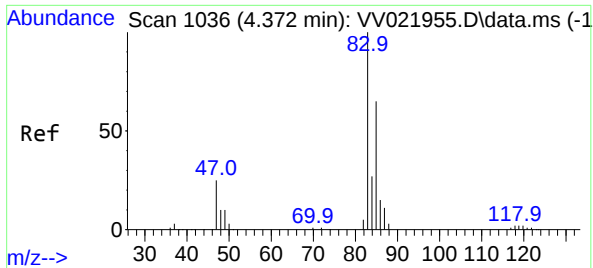

#25
Chloroform
Concen: 2.278 ug/L
RT: 4.381 min Scan# 1039
Delta R.T. 0.009 min
Lab File: VV021956.D
Acq: 26 Aug 2021 10:35

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Tgt Ion: 83 Resp: 12067
Ion Ratio Lower Upper
83 100
85 69.3 44.8 83.2

