

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082621\
 Data File : VV021957.D
 Acq On : 26 Aug 2021 11:37
 Operator : SY/MD
 Sample : VV0826WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK240

Quant Time: Aug 27 03:48:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 27 03:46:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	394951	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	374049	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	199954	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	114539	37.097	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.200%		
7) Chloroethane-d5	1.564	69	98045	42.080	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.160%		
11) 1,1-Dichloroethene-d2	2.104	63	156077	31.757	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.520%		
21) 2-Butanone-d5	3.870	46	197083	102.632	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.630%		
24) Chloroform-d	4.346	84	239930	44.852	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.700%		
26) 1,2-Dichloroethane-d4	5.030	65	152512	49.565	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.120%		
32) Benzene-d6	5.047	84	524143	48.729	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.460%		
36) 1,2-Dichloropropane-d6	6.069	67	166890	49.824	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.640%		
41) Toluene-d8	7.317	98	488995	49.185	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.380%		
43) trans-1,3-Dichloroprop...	7.622	79	75165	45.596	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.200%		
47) 2-Hexanone-d5	8.088	63	119235	108.609	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	108.610%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	199921	48.163	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.320%		
66) 1,2-Dichlorobenzene-d4	11.625	152	204692	49.465	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.940%		
Target Compounds					Qvalue	
25) Chloroform	4.378	83	12592	2.400	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082621\
Data File : VV021957.D
Acq On : 26 Aug 2021 11:37
Operator : SY/MD
Sample : VV0826WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK240

Quant Time: Aug 27 03:48:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 27 03:46:52 2021
Response via : Initial Calibration

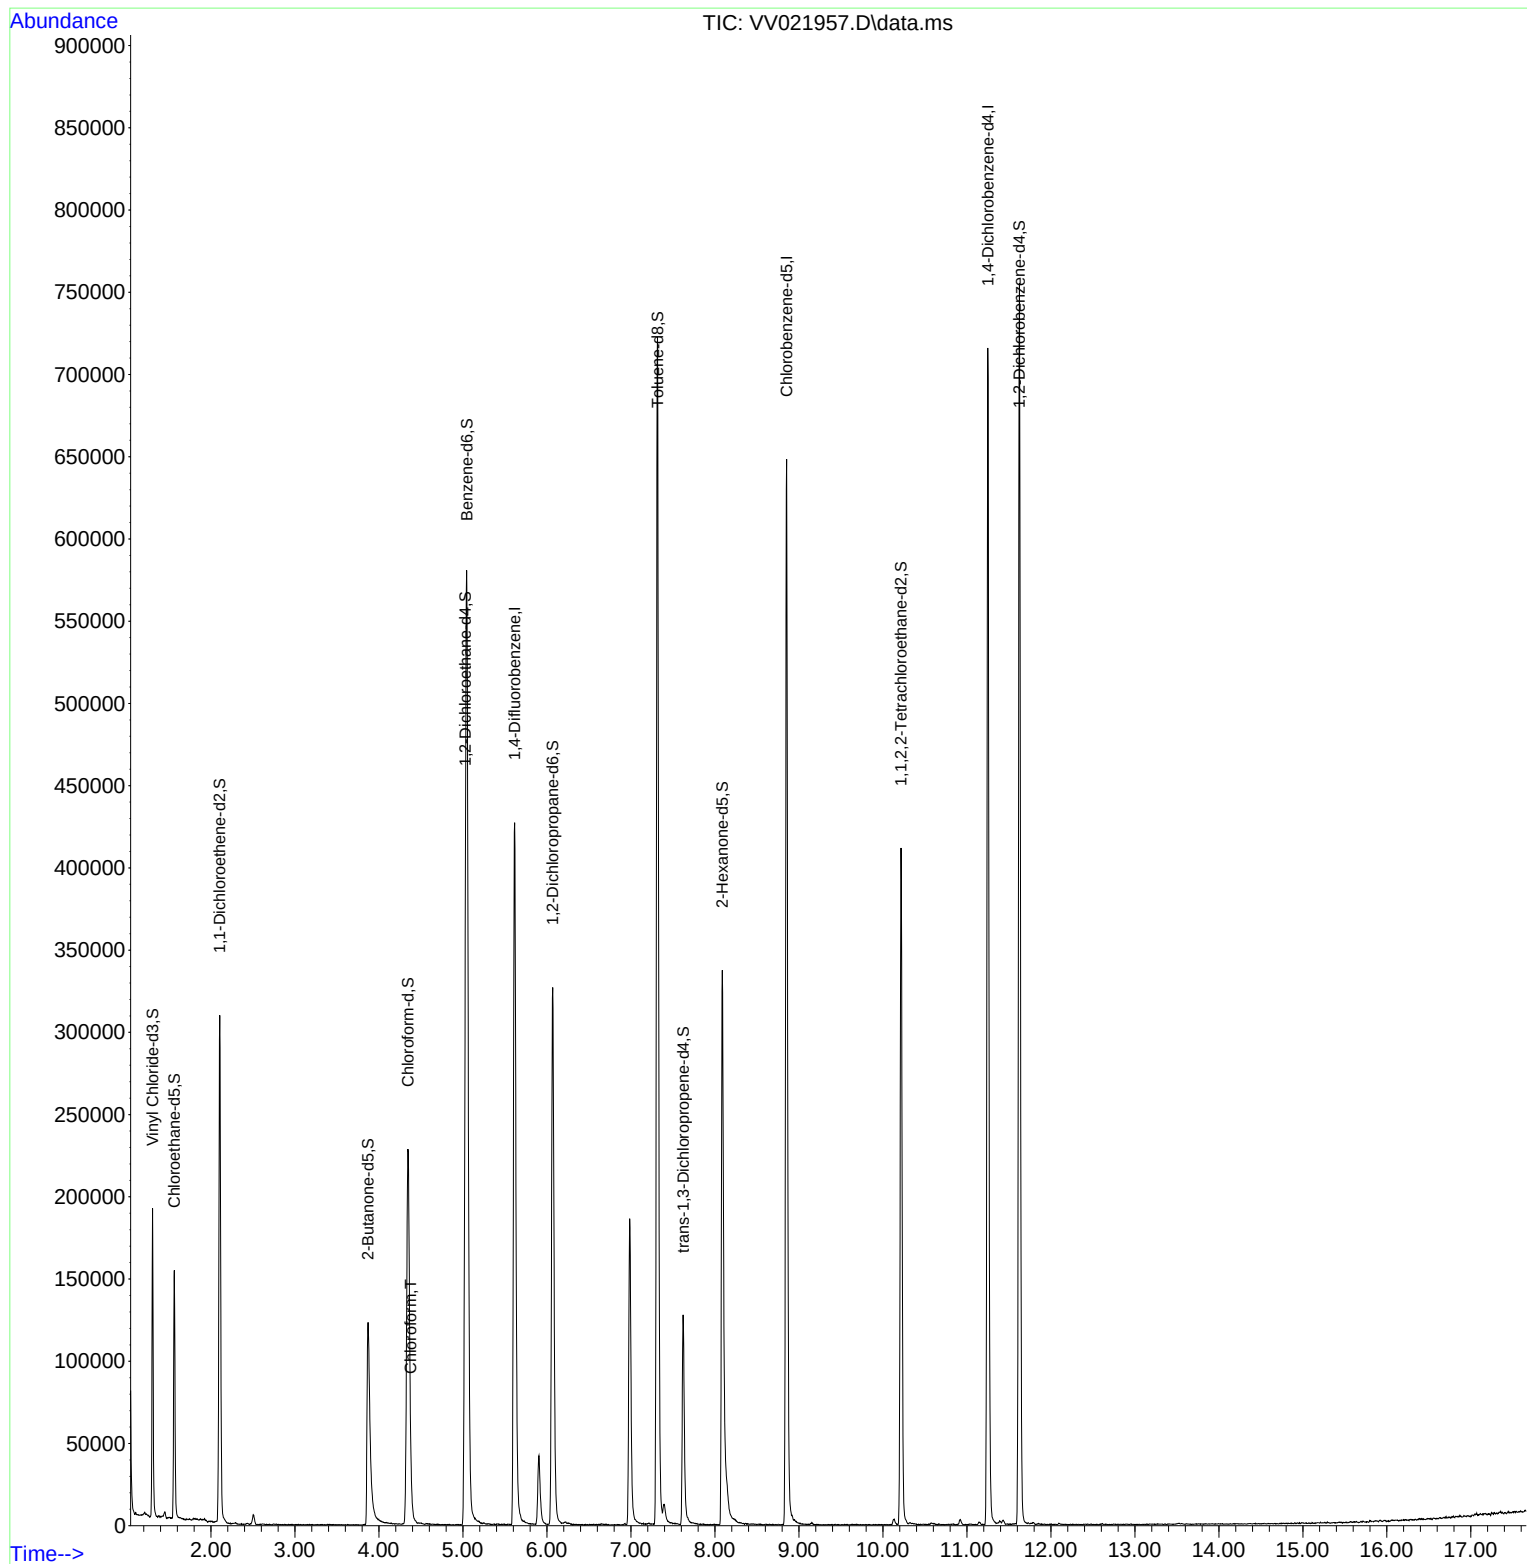

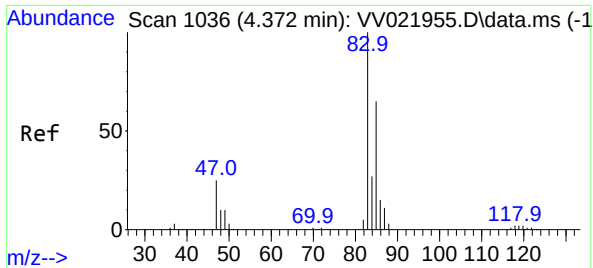

#25
Chloroform
Concen: 2.400 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VV021957.D
Acq: 26 Aug 2021 11:37

Instrument :
MSVOA_V
ClientSampleId :
VBLK240

Tgt Ion: 83 Resp: 12592
Ion Ratio Lower Upper
83 100
85 66.9 44.8 83.2

