


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082621\
 Data File : VV021954.D
 Acq On : 26 Aug 2021 09:09
 Operator : SY/MD
 Sample : BFB222
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB222

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM081621WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 27 03:46:52 2021

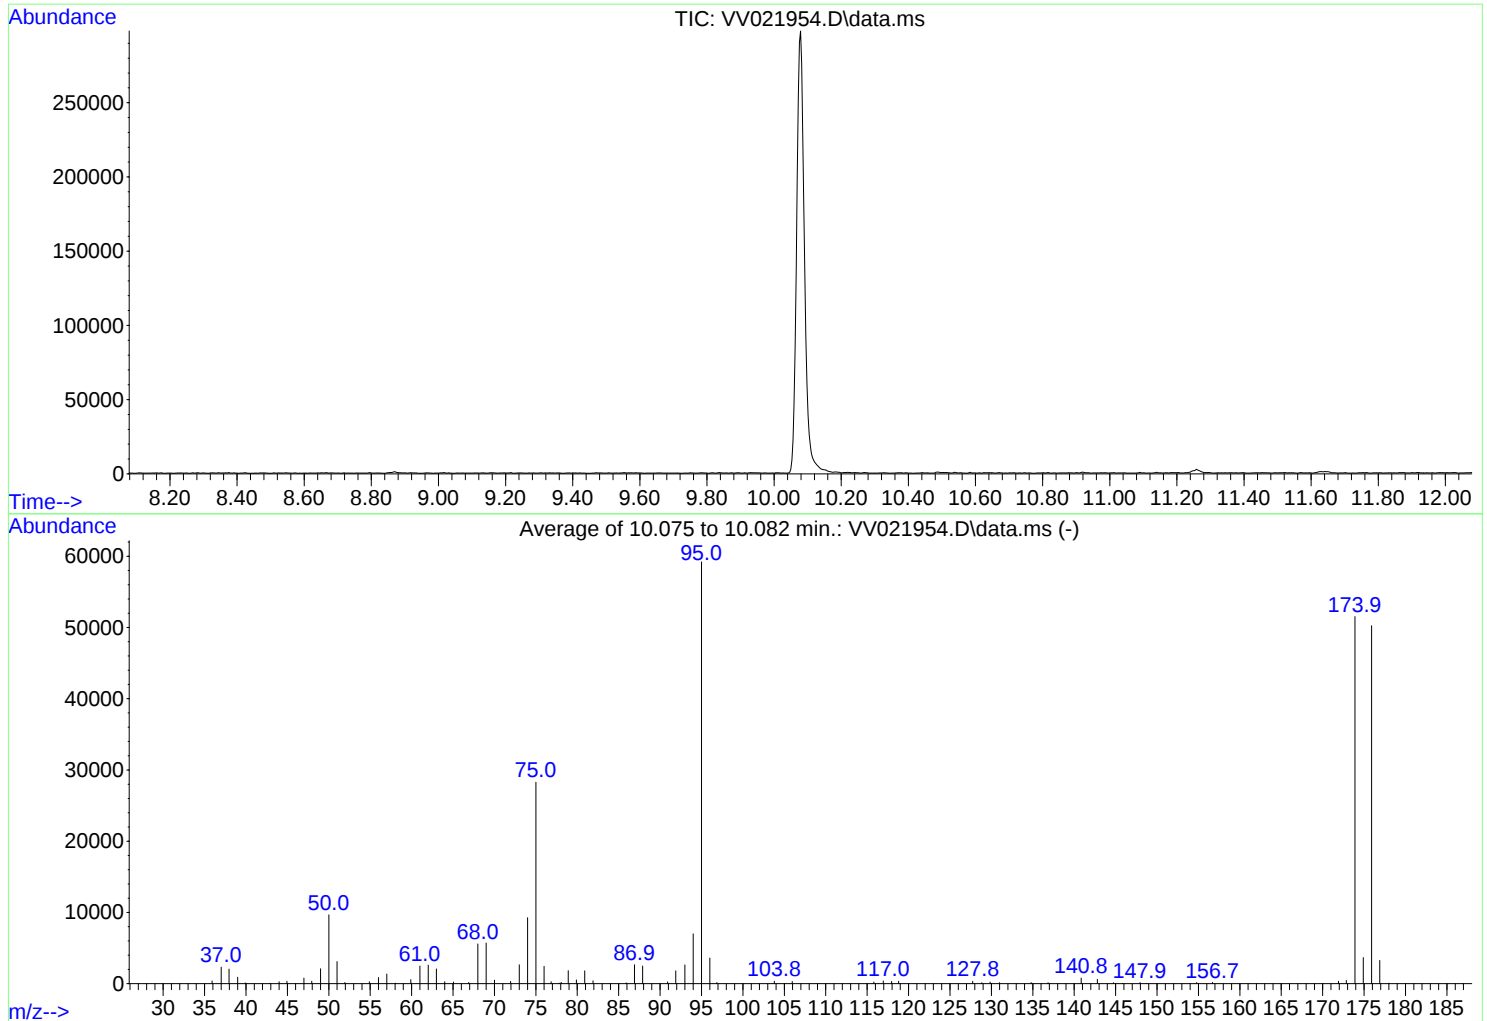

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9654	PASS
75	95	30	80	47.7	28275	PASS
95	95	100	100	100.0	59219	PASS
96	95	5	9	6.1	3604	PASS
173	174	0.00	2	0.9	448	PASS
174	95	50	120	87.0	51533	PASS
175	174	5	9	7.1	3659	PASS
176	174	95	105	97.5	50248	PASS
177	176	5	10	6.5	3262	PASS

Scan 2799 (10.040 min): VV021954.D\data.ms
BFB222

m/z	Abundance
40.00	174.0
44.00	327.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.90	390.0
37.00	2394.0
38.00	2039.0
39.00	924.0
39.80	259.0
44.00	616.0
45.00	348.0
46.00	105.0
47.00	804.0
47.90	340.0
49.00	2285.0
50.00	9794.0
51.00	3210.0
51.90	137.0
54.90	232.0
56.00	937.0
57.00	1418.0
59.90	593.0
61.00	2493.0
62.00	2583.0
63.00	2111.0
64.00	253.0
65.10	221.0
66.80	182.0
68.00	5748.0
69.00	5976.0
70.00	478.0
72.00	282.0
73.00	2734.0
74.00	9777.0
75.00	29080.0
76.00	2515.0
76.80	318.0
77.80	227.0
78.90	1918.0
79.90	511.0
80.90	1714.0
81.90	378.0
85.90	121.0
86.90	2539.0
87.90	2487.0
90.90	219.0
91.90	1870.0
93.00	2628.0
94.00	7159.0
95.00	60264.0
96.00	3699.0
96.90	157.0
103.80	363.0
105.90	291.0
115.80	218.0
117.00	414.0
117.90	328.0
118.80	354.0
127.70	373.0
128.90	166.0
129.80	226.0
131.00	119.0
134.80	143.0
136.80	105.0
140.90	766.0
142.80	638.0
144.70	150.0
148.00	159.0
148.70	101.0
154.80	167.0
156.70	167.0
171.90	353.0
173.00	476.0
173.90	50728.0
174.90	3503.0
175.90	49368.0
176.90	3392.0
178.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.90	398.0
37.00	2429.0
37.90	2144.0
39.00	930.0
39.90	282.0
44.00	605.0
45.00	342.0
47.00	827.0
48.00	349.0
49.00	2111.0
50.00	9962.0
51.00	3209.0
52.00	155.0
54.90	290.0
56.00	867.0
57.00	1359.0
58.10	105.0
59.90	594.0
61.00	2535.0
62.00	2617.0
63.00	2110.0
64.00	279.0
65.00	223.0
66.90	151.0
68.00	5744.0
69.00	5930.0
70.00	521.0
72.00	331.0
73.00	2739.0
74.00	9593.0
75.00	29504.0
76.00	2465.0
76.80	279.0
78.10	274.0
78.90	1845.0
79.90	535.0
80.90	1883.0
81.90	409.0
85.90	137.0
86.90	2762.0
87.90	2540.0
90.90	277.0
91.90	1890.0
93.00	2731.0
94.00	7197.0
95.00	61232.0
96.00	3707.0
96.90	164.0
103.80	339.0
105.90	332.0
115.80	243.0
116.90	390.0
118.00	331.0
118.80	339.0
127.70	368.0
128.80	138.0
129.90	215.0
131.00	153.0
134.80	165.0
136.90	143.0
140.90	823.0
142.80	599.0
144.80	144.0
148.00	168.0
154.80	160.0
156.70	202.0
171.90	363.0
172.80	475.0
173.90	53280.0
174.90	3792.0
175.90	52096.0
176.90	3365.0
178.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.90	361.0
37.00	2133.0
38.00	1922.0
39.00	843.0
39.90	311.0
42.90	118.0
44.00	575.0
44.90	346.0
47.00	723.0
48.00	340.0
49.00	1854.0
50.00	9205.0
51.00	2870.0
51.90	180.0
54.90	272.0
56.00	762.0
57.00	1262.0
58.00	115.0
59.90	514.0
61.00	2397.0
62.00	2629.0
63.00	1962.0
64.00	253.0
65.00	231.0
67.00	124.0
68.00	5211.0
69.00	5243.0
70.00	492.0
71.90	362.0
73.00	2465.0
74.00	8417.0
75.00	26240.0
76.00	2295.0
76.90	222.0
78.00	271.0
78.90	1699.0
79.90	511.0
80.90	1826.0
81.90	426.0
85.90	115.0
86.90	2635.0
87.90	2419.0
90.90	254.0
91.90	1618.0
93.00	2511.0
94.00	6621.0
95.00	56160.0
96.00	3406.0
96.80	148.0
103.80	315.0
106.00	308.0
115.80	227.0
116.90	367.0
117.90	278.0
118.80	327.0
127.80	281.0
128.80	113.0
129.90	217.0
131.00	146.0
134.80	166.0
136.90	134.0
140.80	784.0
142.80	559.0
144.80	117.0
145.80	113.0
147.90	158.0
154.80	133.0
156.70	163.0
171.90	320.0
172.80	394.0
173.90	50592.0
174.90	3683.0
175.90	49280.0
176.90	3029.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222