

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027528.D
 Acq On : 26 Aug 2022 12:17
 Operator : SY/MD
 Sample : VV0826WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Quant Time: Aug 27 03:13:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 27 03:12:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	131288	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	126858	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	55433	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	41373	4.428	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.600%
7) Chloroethane-d5	1.561	69	38569	5.640	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.800%
11) 1,1-Dichloroethene-d2	2.098	63	70303	3.227	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.600%
20) 2-Butanone-d5	3.902	46	54576	46.934	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.860%
24) Chloroform-d	4.343	84	78412	4.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	5.031	65	38796	4.800	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.000%
32) Benzene-d6	5.044	84	146215	4.161	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.200%
36) 1,2-Dichloropropane-d6	6.066	67	43284	4.237	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.800%
41) Toluene-d8	7.314	98	117244	3.695	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.000%
43) trans-1,3-Dichloroprop...	7.625	79	13550	3.874	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.400%
46) 2-Hexanone-d5	8.088	63	48605	42.213	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.420%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	27749	4.265	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	39990	4.867	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.400%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	12963	0.866	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027528.D
Acq On : 26 Aug 2022 12:17
Operator : SY/MD
Sample : VV0826WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Time: Aug 27 03:13:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 27 03:12:26 2022
Response via : Initial Calibration

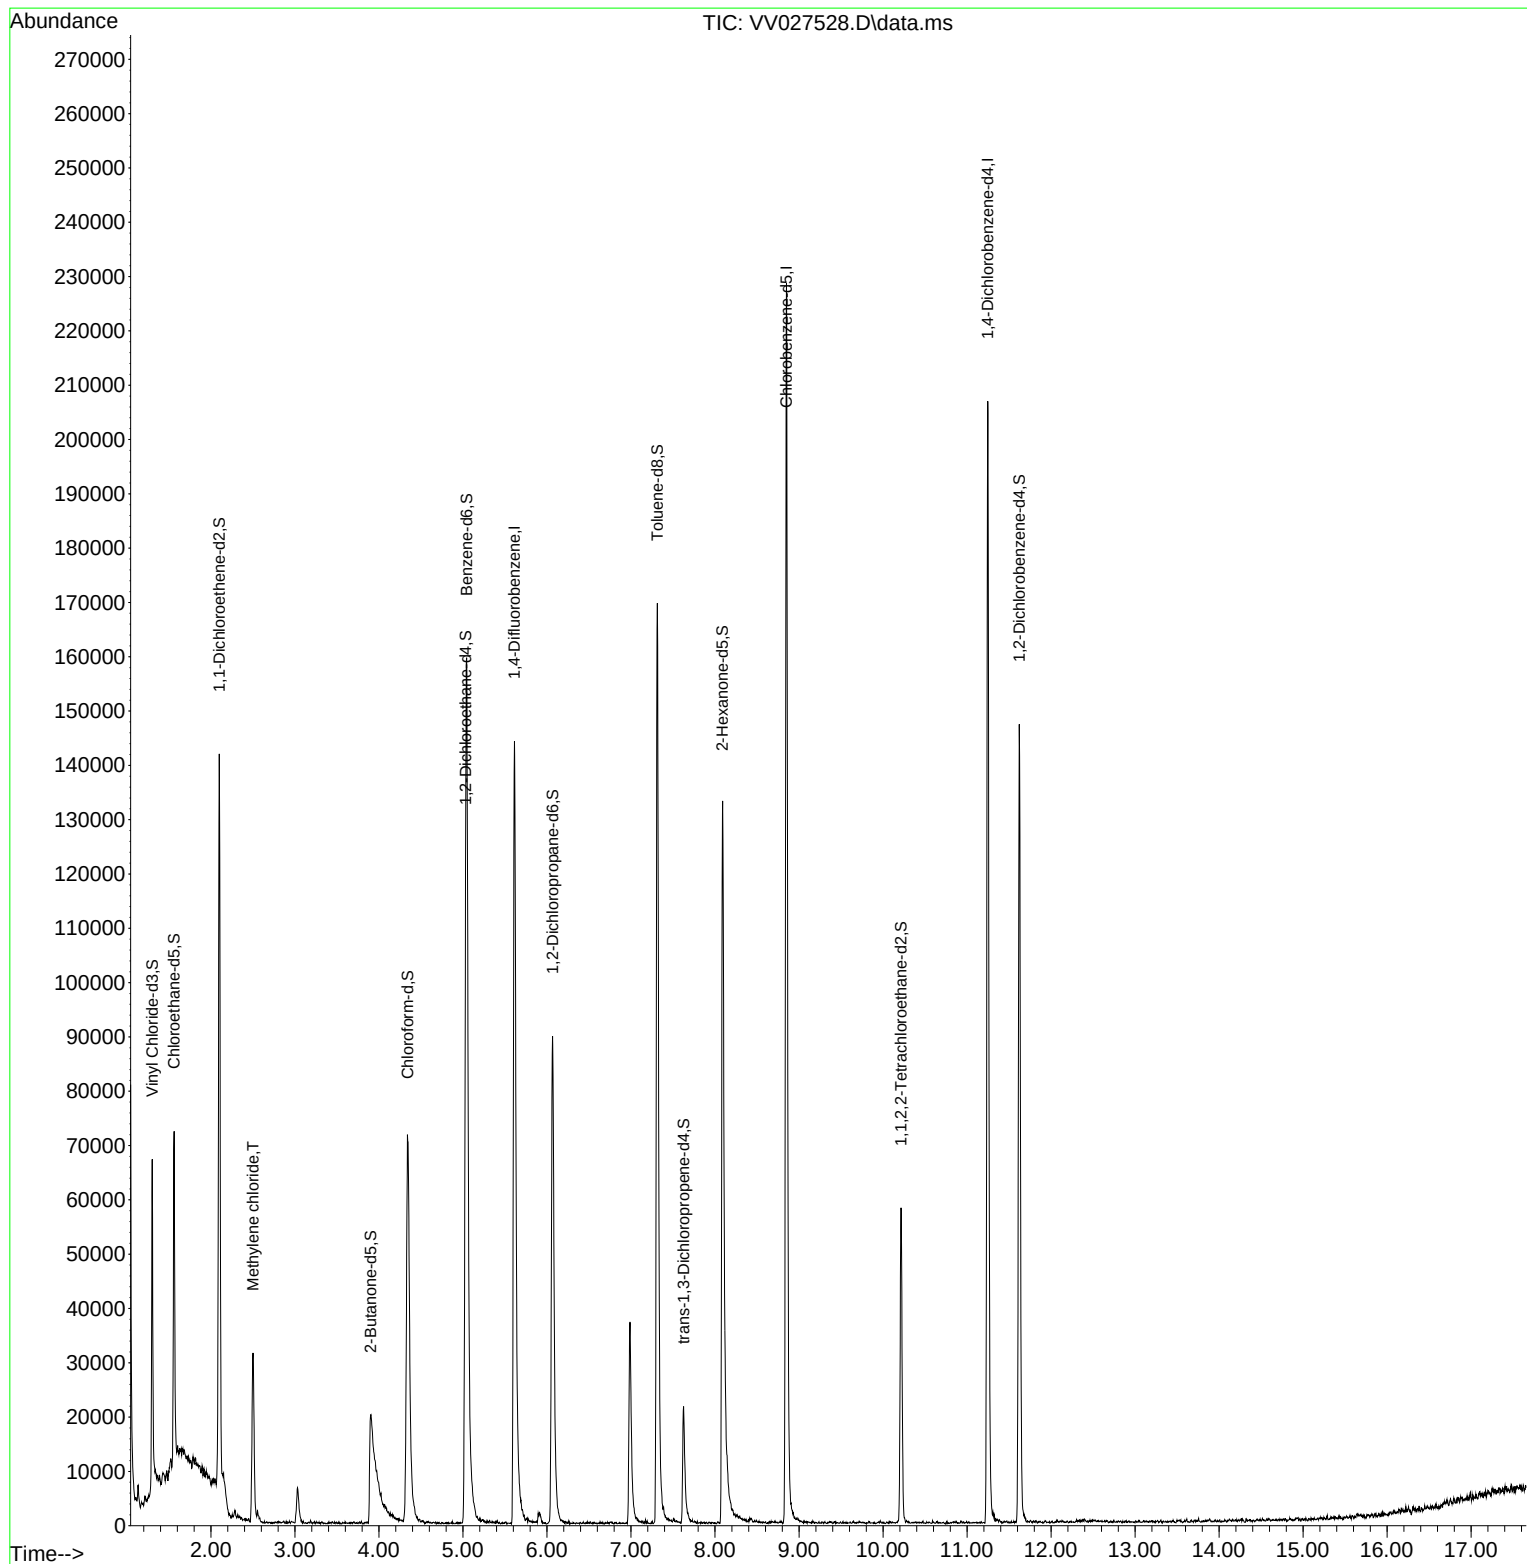

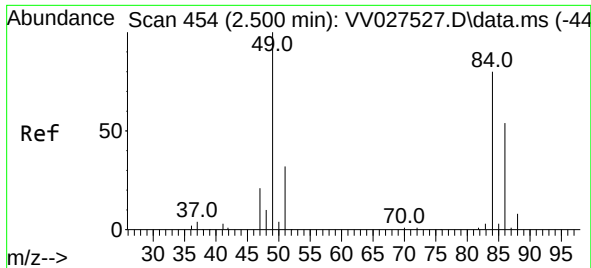

#16
Methylene chloride
Concen: 0.866 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV027528.D
Acq: 26 Aug 2022 12:17

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Tgt Ion: 84	Resp:	12963
Ion	Ratio	Lower Upper
84	100	
86	64.0	44.0 81.6
49	121.4	89.4 166.0

