

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027545.D
 Acq On : 26 Aug 2022 19:43
 Operator : SY/MD
 Sample : N4368-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F05

Quant Time: Aug 27 03:17:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 27 03:12:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	128916	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	128117	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55524	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	33264	3.625	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.564	69	33720	5.022	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.400%
11) 1,1-Dichloroethene-d2	2.105	63	64263	3.004	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.000%
20) 2-Butanone-d5	3.896	46	41506	36.351	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.700%
24) Chloroform-d	4.346	84	76005	4.143	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.800%
26) 1,2-Dichloroethane-d4	5.034	65	38419	4.841	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.800%
32) Benzene-d6	5.047	84	139444	3.930	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.600%
36) 1,2-Dichloropropane-d6	6.069	67	42950	4.163	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.200%
41) Toluene-d8	7.317	98	112926	3.524	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.400%
43) trans-1,3-Dichloroprop...	7.625	79	12167	3.444	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.800%
46) 2-Hexanone-d5	8.091	63	49777	42.807	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.620%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31408	4.780	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	39406	4.788	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.800%
Target Compounds					Qvalue	
30) Cyclohexane	4.667	56	2739	0.181	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027545.D
Acq On : 26 Aug 2022 19:43
Operator : SY/MD
Sample : N4368-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F05

Quant Time: Aug 27 03:17:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 27 03:12:26 2022
Response via : Initial Calibration

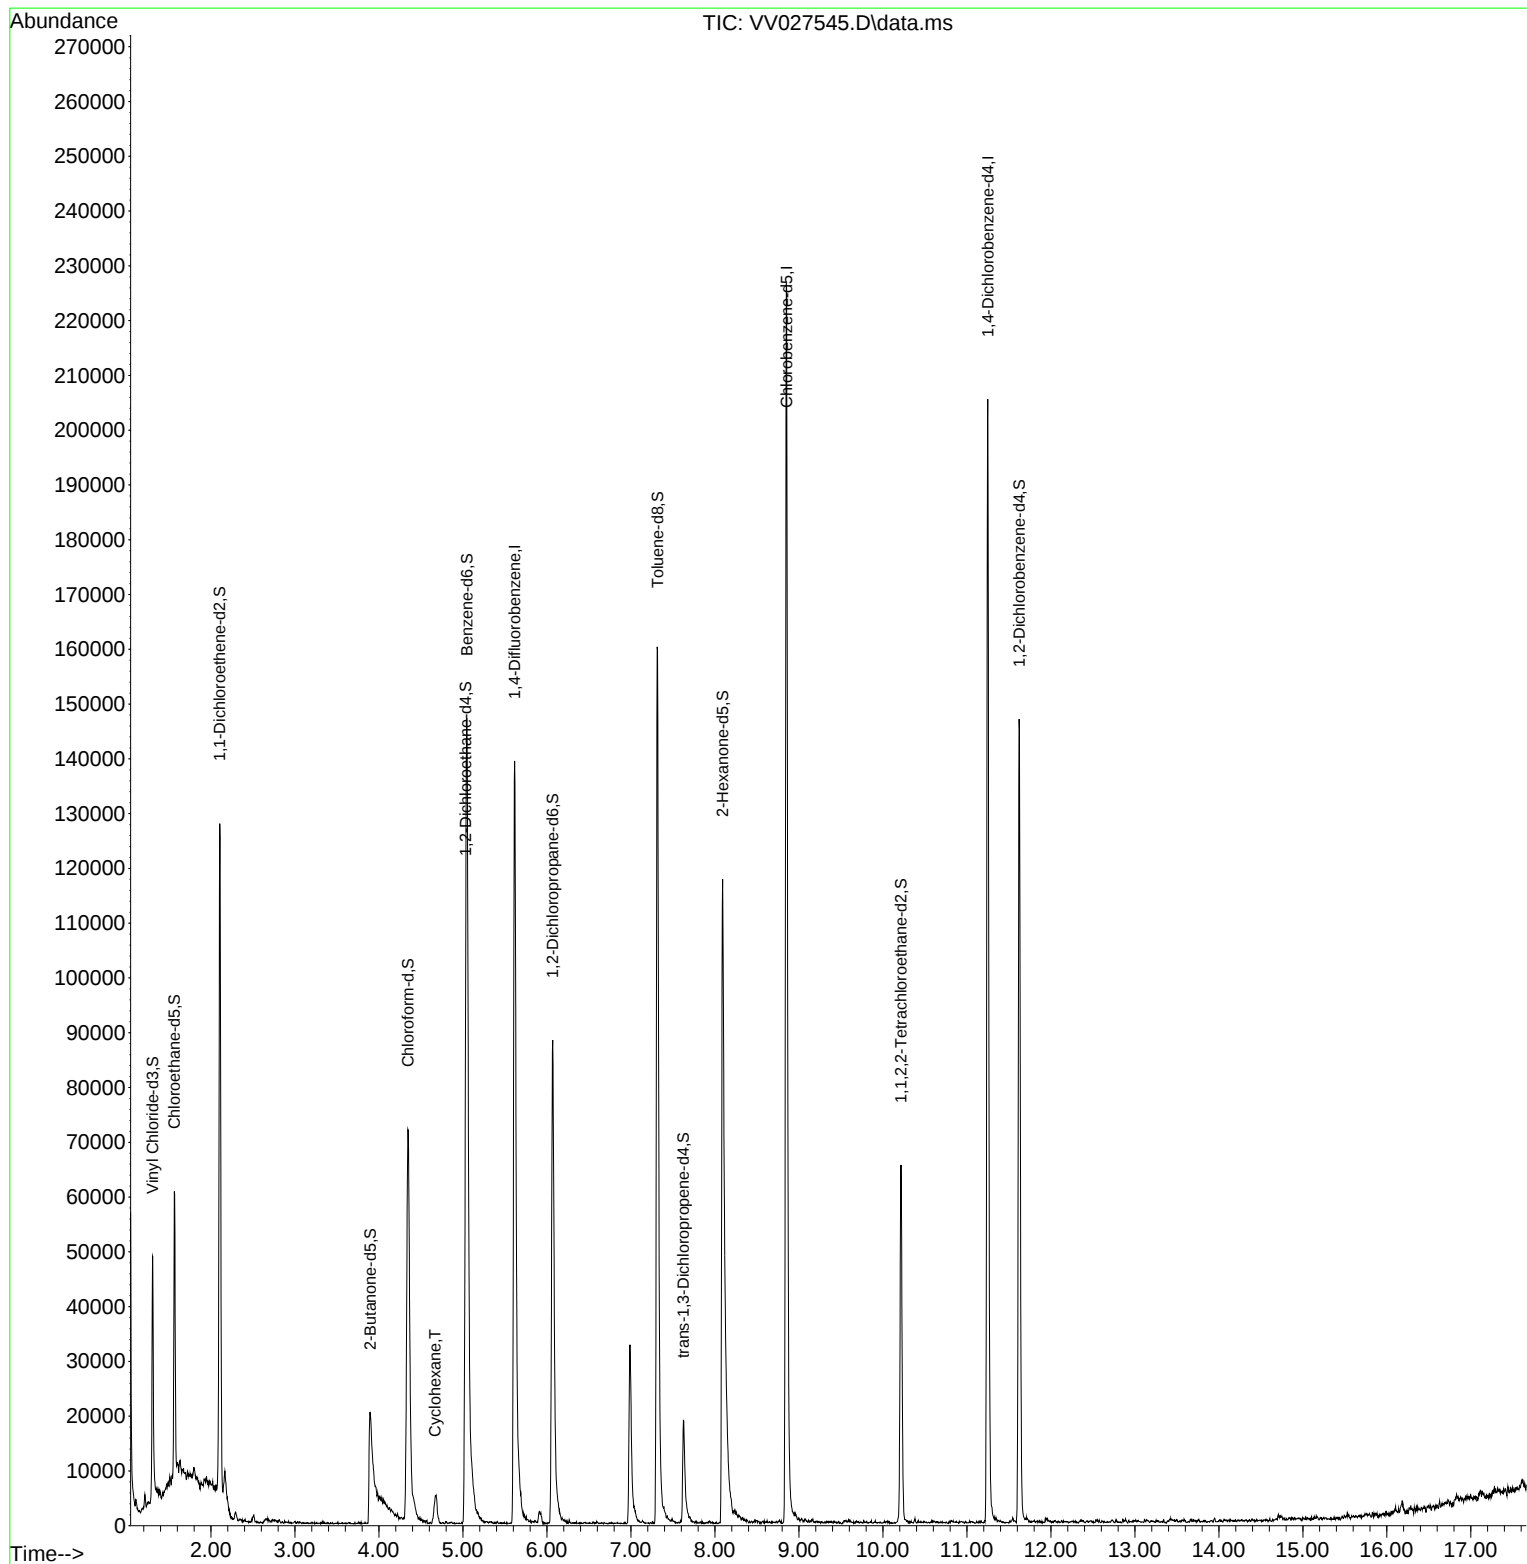

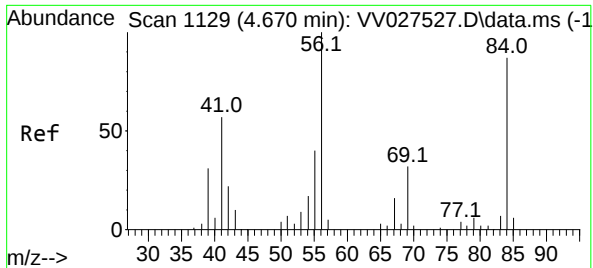

#30
Cyclohexane
Concen: 0.181 ug/L
RT: 4.667 min Scan# 11
Delta R.T. -0.003 min
Lab File: VV027545.D
Acq: 26 Aug 2022 19:43

Instrument :
MSVOA_V
ClientSampleId :
F5F05

Tgt Ion: 56	Resp:	2739
Ion	Ratio	Lower Upper
56	100	
69	19.0	25.4 38.0#
84	55.3	69.7 104.5#

