

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027528.D
 Acq On : 26 Aug 2022 12:17
 Operator : SY/MD
 Sample : VV0826WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	25	29	37	rVB2	4171	4584	1.12%	0.137%
2	1.301	74	81	91	rBV	60951	64204	15.75%	1.918%
3	1.561	155	162	172	rBV	60831	69984	17.17%	2.090%
4	2.098	318	329	343	rBV	134595	192674	47.28%	5.755%
5	2.500	443	454	468	rBV	31176	54060	13.26%	1.615%
6	3.031	609	619	632	rBV4	6492	12957	3.18%	0.387%
7	3.905	881	891	911	rBV	20041	76631	18.80%	2.289%
8	4.339	1011	1026	1067	rBV	71260	195028	47.85%	5.825%
9	5.044	1229	1245	1281	rBV3	159310	407556	100.00%	12.173%
10	5.613	1411	1422	1450	rBV	144101	313361	76.89%	9.359%
11	6.066	1545	1563	1593	rBV2	89768	199595	48.97%	5.961%
12	6.989	1840	1850	1871	rBV2	36991	74460	18.27%	2.224%
13	7.314	1935	1951	1971	rBV	169489	311773	76.50%	9.312%
14	7.625	2038	2048	2063	rBV	21550	41128	10.09%	1.228%
15	8.092	2182	2193	2226	rBV	133058	283069	69.46%	8.455%
16	8.850	2415	2429	2452	rBV	228356	381193	93.53%	11.385%
17	10.214	2843	2853	2870	rVB2	57913	93039	22.83%	2.779%
18	11.246	3163	3174	3192	rBV	206614	330710	81.14%	9.878%
19	11.622	3280	3291	3317	rVB	146855	242093	59.40%	7.231%




Sum of corrected areas: 3348099

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027528.D
Acq On : 26 Aug 2022 12:17
Operator : SY/MD
Sample : VV0826WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

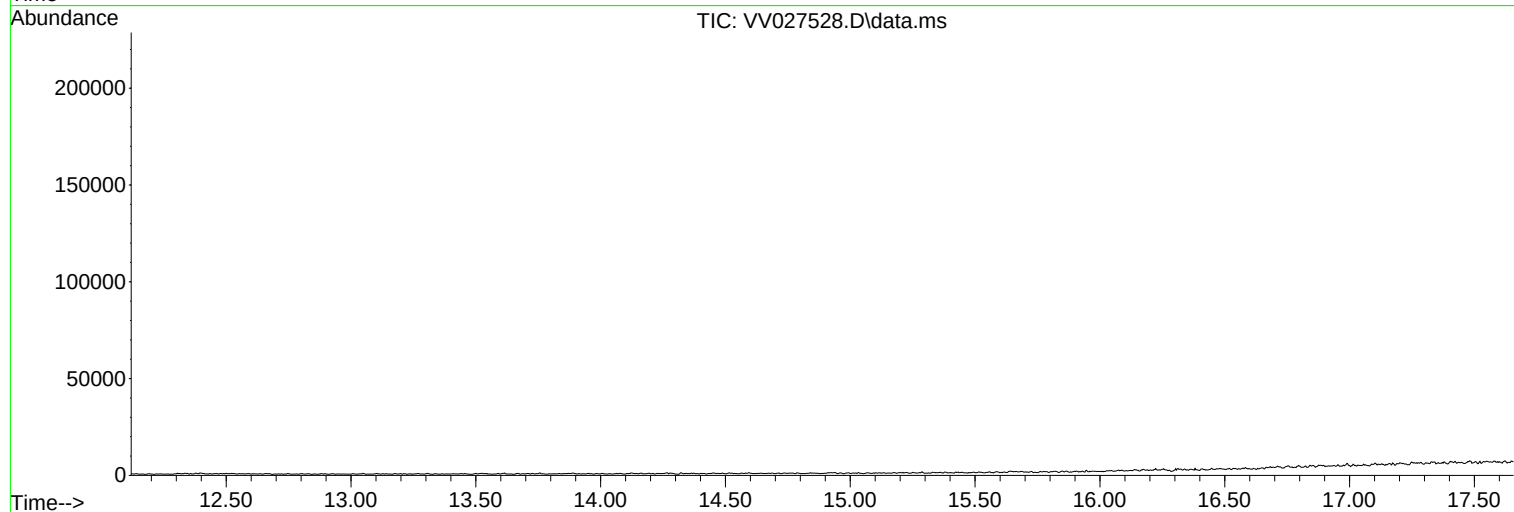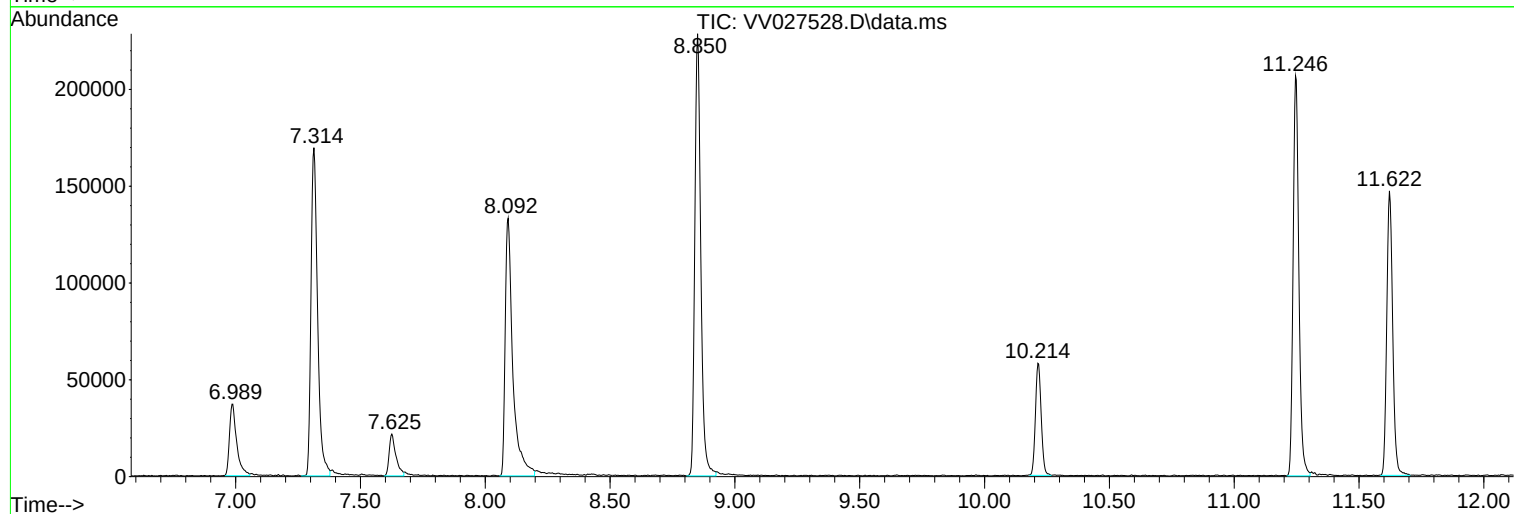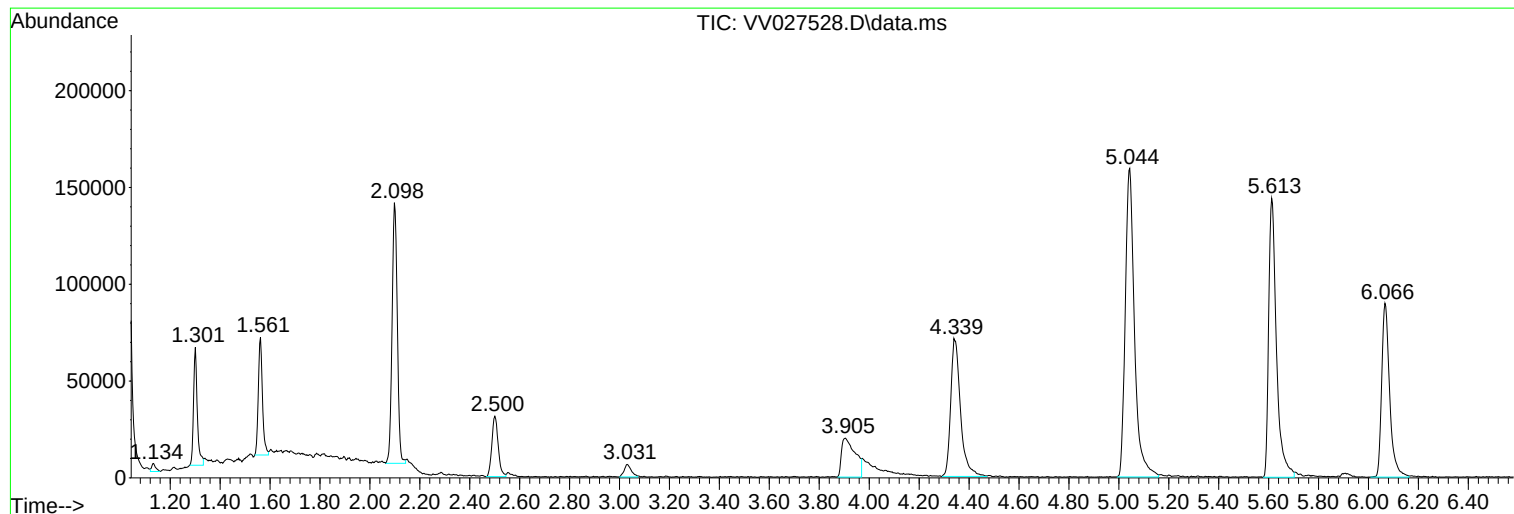

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027528.D
Acq On : 26 Aug 2022 12:17
Operator : SY/MD
Sample : VV0826WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027528.D
Acq On : 26 Aug 2022 12:17
Operator : SY/MD
Sample : VV0826WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
