

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027529.D
 Acq On : 26 Aug 2022 12:44
 Operator : SY/MD
 Sample : N4367-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F26

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	97	rBV	47164	55508	13.95%	1.511%
2	1.564	156	163	177	rBV	55262	68082	17.11%	1.853%
3	2.105	321	331	343	rVB	118755	170048	42.74%	4.629%
4	2.503	445	455	465	rVB3	6473	10675	2.68%	0.291%
5	3.040	612	622	631	rBV6	3310	6013	1.51%	0.164%
6	3.895	878	888	908	rBV	21313	66836	16.80%	1.819%
7	4.346	1011	1028	1059	rBV2	74523	205963	51.77%	5.606%
8	5.043	1229	1245	1285	rBV3	147724	393762	98.97%	10.719%
9	5.612	1411	1422	1459	rBV	144696	318878	80.15%	8.680%
10	5.915	1506	1516	1533	rBV7	9921	22722	5.71%	0.619%
11	6.066	1549	1563	1597	rBV	88274	194618	48.92%	5.298%
12	6.989	1840	1850	1871	rBV	35500	71398	17.95%	1.944%
13	7.313	1941	1951	1978	rBV	159192	299416	75.26%	8.150%
14	7.628	2038	2049	2072	rBV2	20060	42013	10.56%	1.144%
15	7.972	2135	2156	2180	rBV	224608	391383	98.38%	10.654%
16	8.091	2184	2193	2229	rBV	114709	283090	71.16%	7.706%
17	8.850	2414	2429	2460	rBV	235406	397840	100.00%	10.830%
18	10.217	2840	2854	2869	rBV	57555	95149	23.92%	2.590%
19	11.249	3163	3175	3195	rBV	214059	339640	85.37%	9.245%
20	11.622	3279	3291	3309	rBV	148587	240631	60.48%	6.550%




Sum of corrected areas: 3673665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027529.D
Acq On : 26 Aug 2022 12:44
Operator : SY/MD
Sample : N4367-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

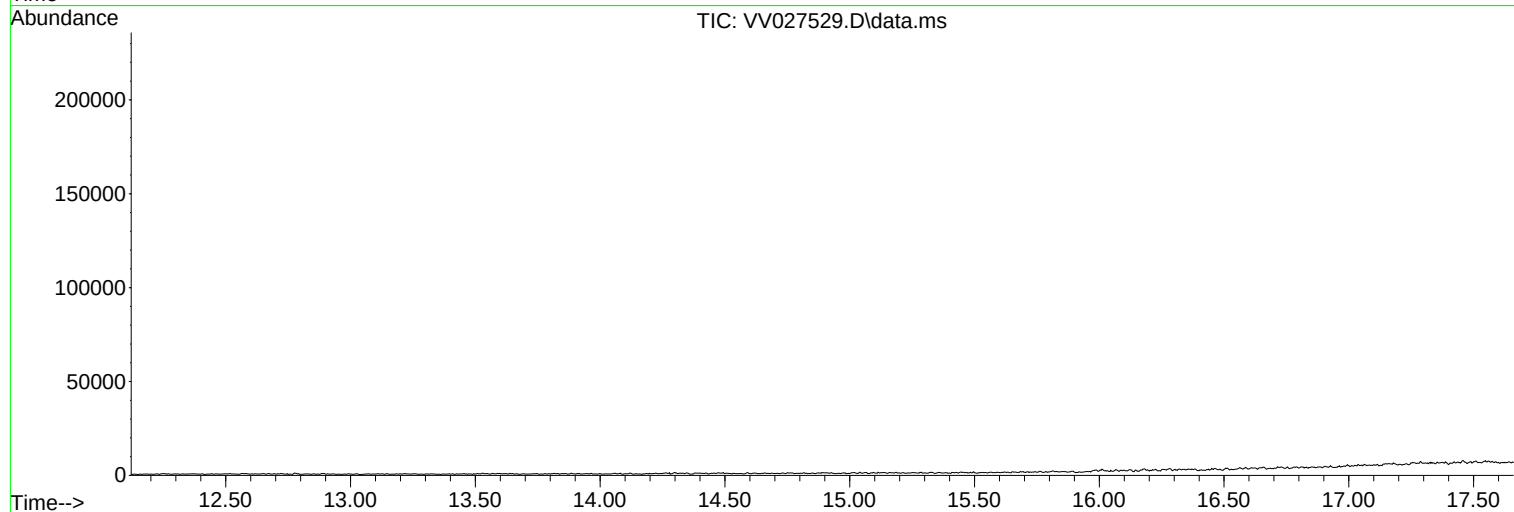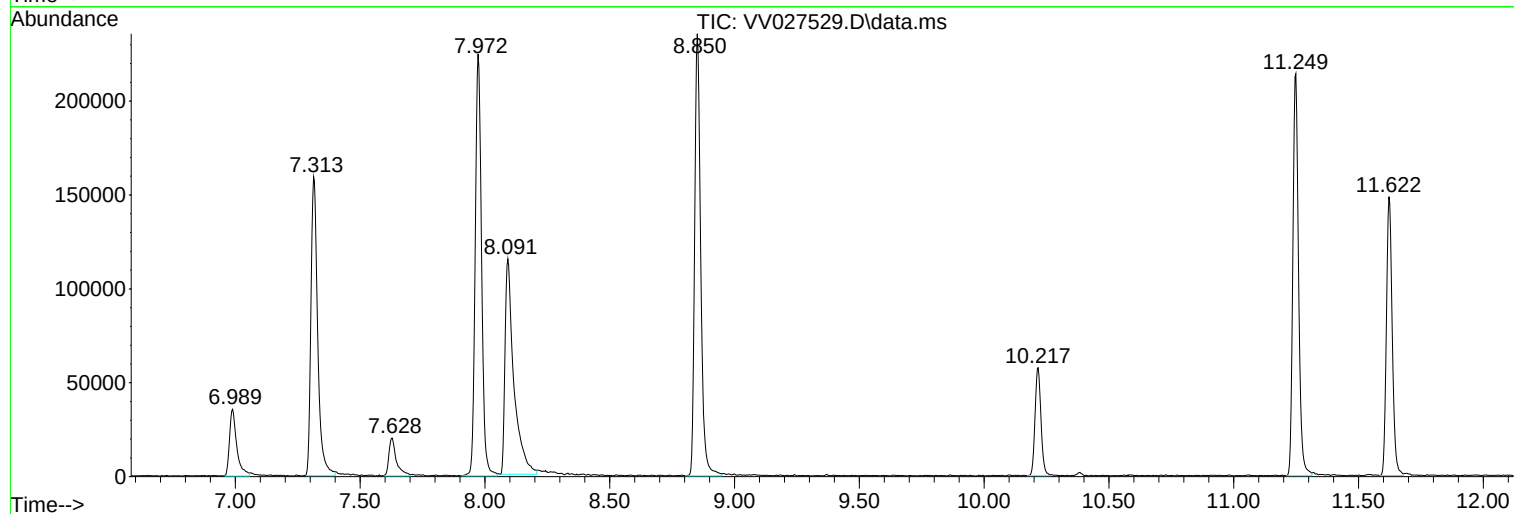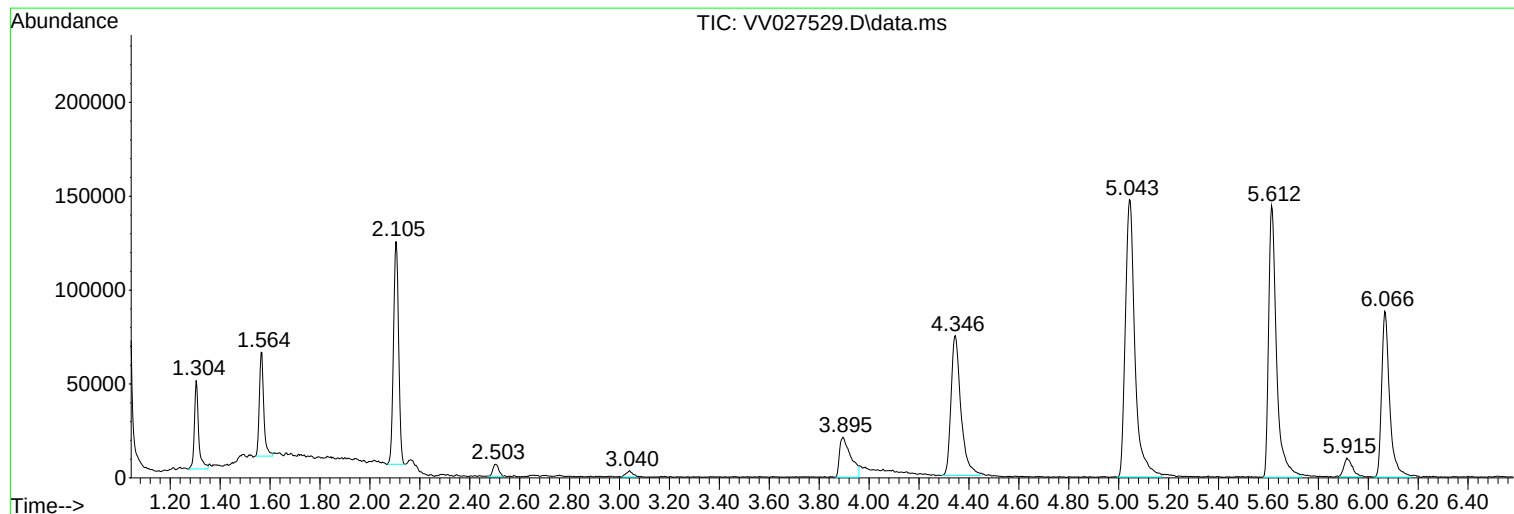

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027529.D
Acq On : 26 Aug 2022 12:44
Operator : SY/MD
Sample : N4367-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027529.D
Acq On : 26 Aug 2022 12:44
Operator : SY/MD
Sample : N4367-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc