

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027534.D
 Acq On : 26 Aug 2022 14:47
 Operator : SY/MD
 Sample : N4368-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E91

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	91	rBV	43990	50203	5.17%	1.080%
2	1.565	157	163	174	rBV	50345	59556	6.13%	1.281%
3	2.105	321	331	343	rVB	122500	177087	18.22%	3.810%
4	2.767	524	537	555	rBV	51430	110766	11.40%	2.383%
5	3.905	879	891	924	rBV3	50904	170273	17.52%	3.663%
6	4.346	1013	1028	1068	rBV2	70013	194428	20.01%	4.183%
7	5.043	1231	1245	1285	rBV2	141690	380658	39.17%	8.189%
8	5.616	1412	1423	1460	rBV	151587	334849	34.46%	7.204%
9	5.915	1503	1516	1549	rBV2	105627	230319	23.70%	4.955%
10	6.069	1552	1564	1588	rBV2	86399	187515	19.30%	4.034%
11	6.989	1840	1850	1873	rBV3	33405	71122	7.32%	1.530%
12	7.317	1939	1952	1972	rBV	155828	290869	29.93%	6.257%
13	7.625	2039	2048	2072	rBV2	19762	39186	4.03%	0.843%
14	7.973	2143	2156	2182	rBV	562853	971720	100.00%	20.904%
15	8.092	2184	2193	2225	rBV	115007	284159	29.24%	6.113%
16	8.850	2419	2429	2458	rBV	243187	412104	42.41%	8.865%
17	10.217	2841	2854	2871	rBV2	58575	96614	9.94%	2.078%
18	11.249	3164	3175	3196	rBV	218178	349560	35.97%	7.520%
19	11.622	3274	3291	3309	rBV2	142750	237432	24.43%	5.108%




Sum of corrected areas: 4648420

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027534.D
Acq On : 26 Aug 2022 14:47
Operator : SY/MD
Sample : N4368-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

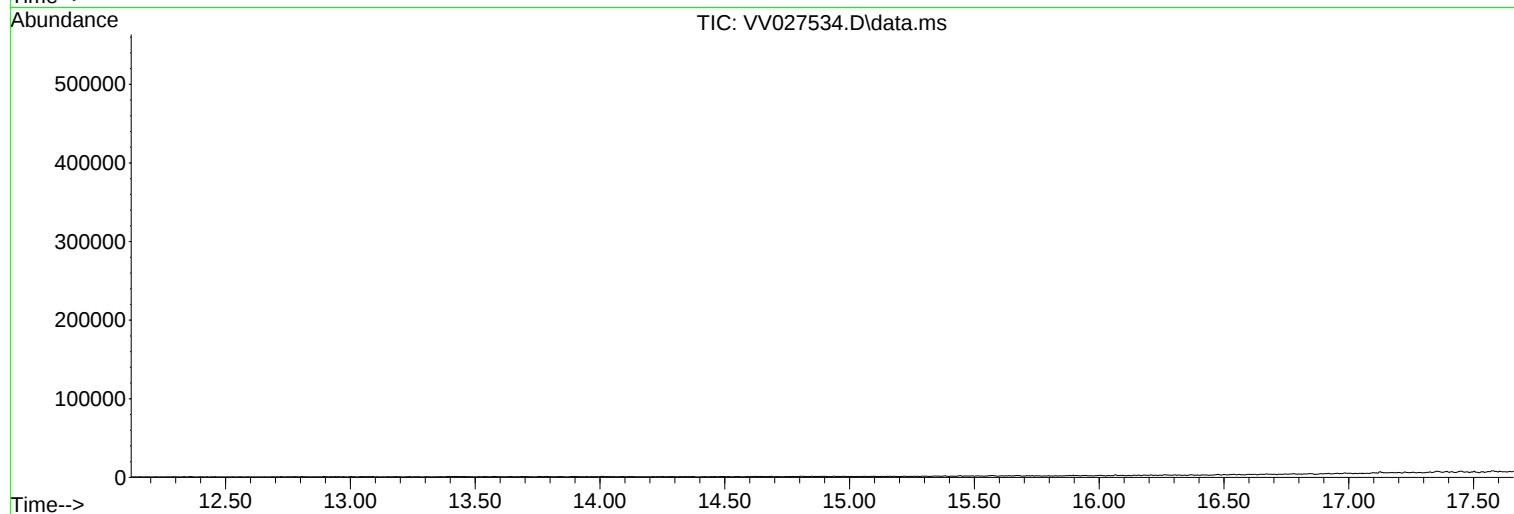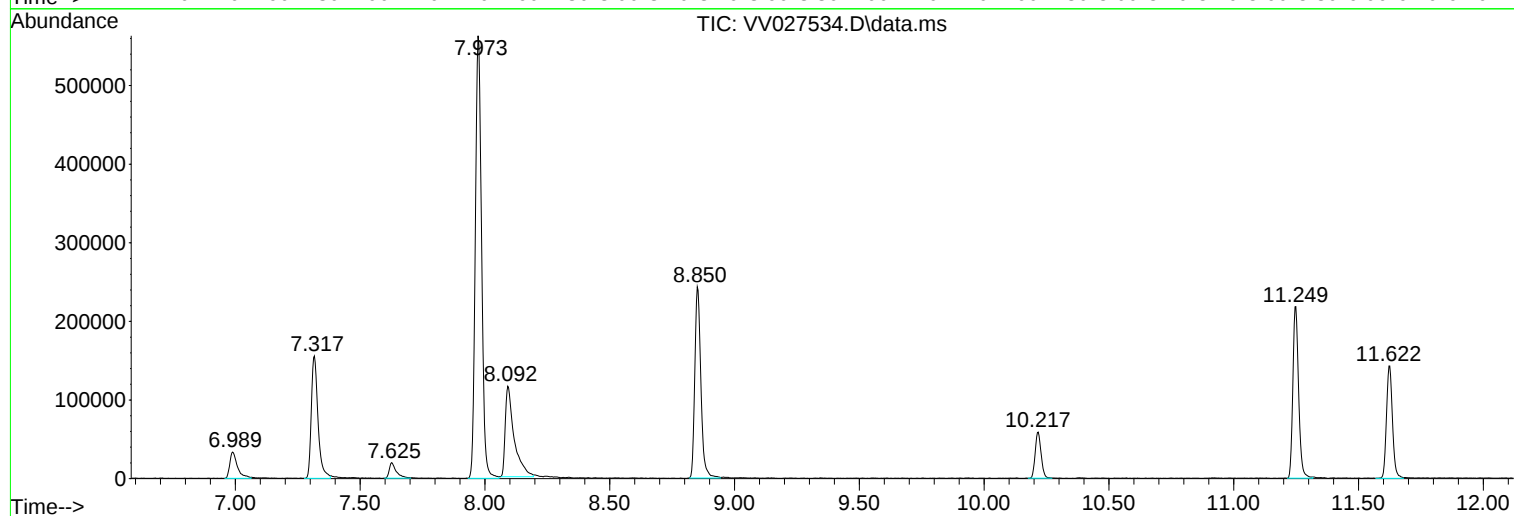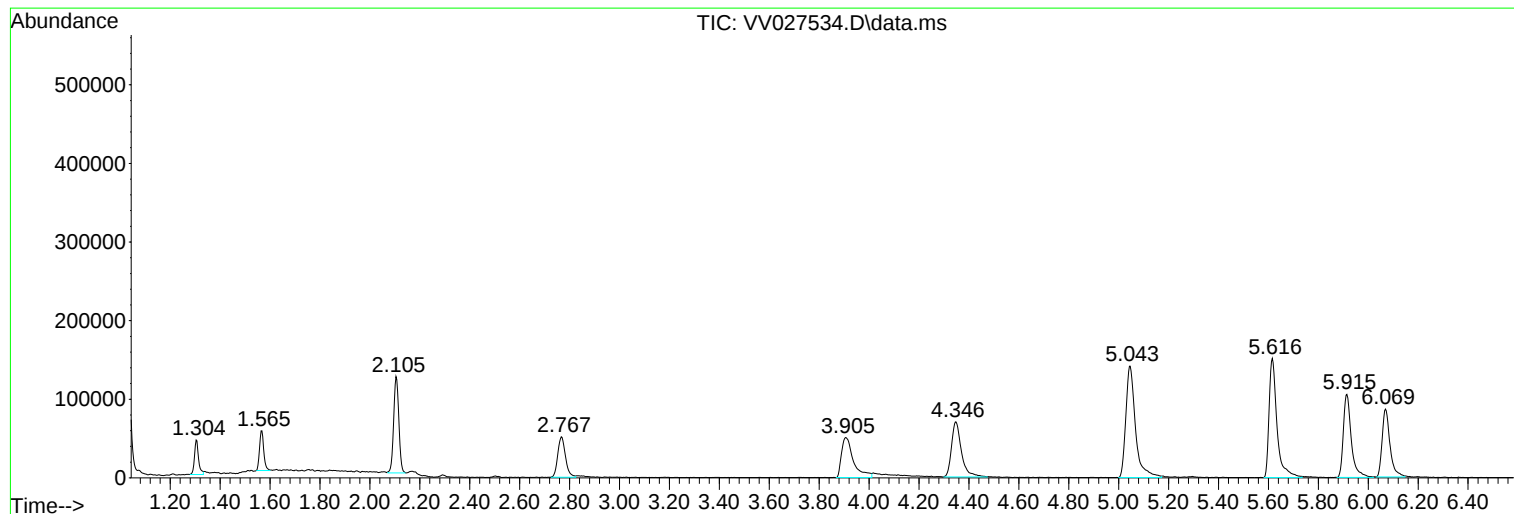

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027534.D
Acq On : 26 Aug 2022 14:47
Operator : SY/MD
Sample : N4368-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027534.D
Acq On : 26 Aug 2022 14:47
Operator : SY/MD
Sample : N4368-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc