

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027537.D
 Acq On : 26 Aug 2022 16:01
 Operator : SY/MD
 Sample : N4368-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5E96

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	72	81	90	rBV	44098	51800	14.08%	1.648%
2	1.565	156	163	175	rBV	48702	56791	15.44%	1.807%
3	2.102	317	330	343	rVB	121039	174035	47.30%	5.536%
4	2.246	369	375	383	rBV4	5062	7087	1.93%	0.225%
5	2.770	525	538	556	rVB2	22851	48151	13.09%	1.532%
6	3.896	878	888	906	rBV2	24352	70513	19.16%	2.243%
7	4.346	1011	1028	1053	rBV2	71323	179743	48.85%	5.718%
8	5.047	1227	1246	1269	rBV2	145835	362588	98.55%	11.534%
9	5.159	1271	1281	1291	rVB5	6328	14549	3.95%	0.463%
10	5.616	1412	1423	1445	rBV	134792	281819	76.60%	8.965%
11	5.915	1507	1516	1529	rVB7	3710	8025	2.18%	0.255%
12	6.069	1552	1564	1582	rBV2	85707	180457	49.05%	5.741%
13	6.140	1582	1586	1603	rVB5	5355	9932	2.70%	0.316%
14	6.989	1837	1850	1880	rBV	32953	69190	18.81%	2.201%
15	7.317	1940	1952	1980	rBV	155277	289562	78.70%	9.211%
16	7.629	2040	2049	2077	rBV2	18789	39772	10.81%	1.265%
17	8.092	2184	2193	2228	rBV	118917	290469	78.95%	9.240%
18	8.850	2415	2429	2452	rBV	213821	367931	100.00%	11.704%
19	10.217	2840	2854	2867	rBV	58394	95082	25.84%	3.025%
20	11.249	3163	3175	3198	rBV	197140	311409	84.64%	9.906%
21	11.625	3281	3292	3308	rBV	143516	234637	63.77%	7.464%




Sum of corrected areas: 3143542

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027537.D
Acq On : 26 Aug 2022 16:01
Operator : SY/MD
Sample : N4368-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

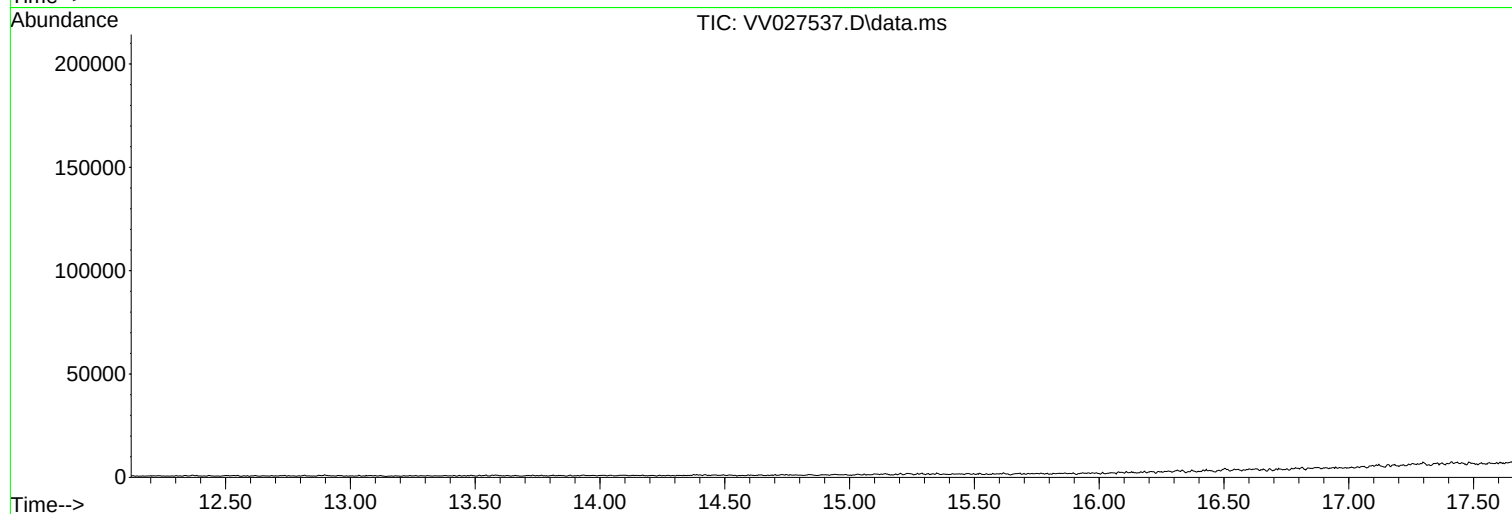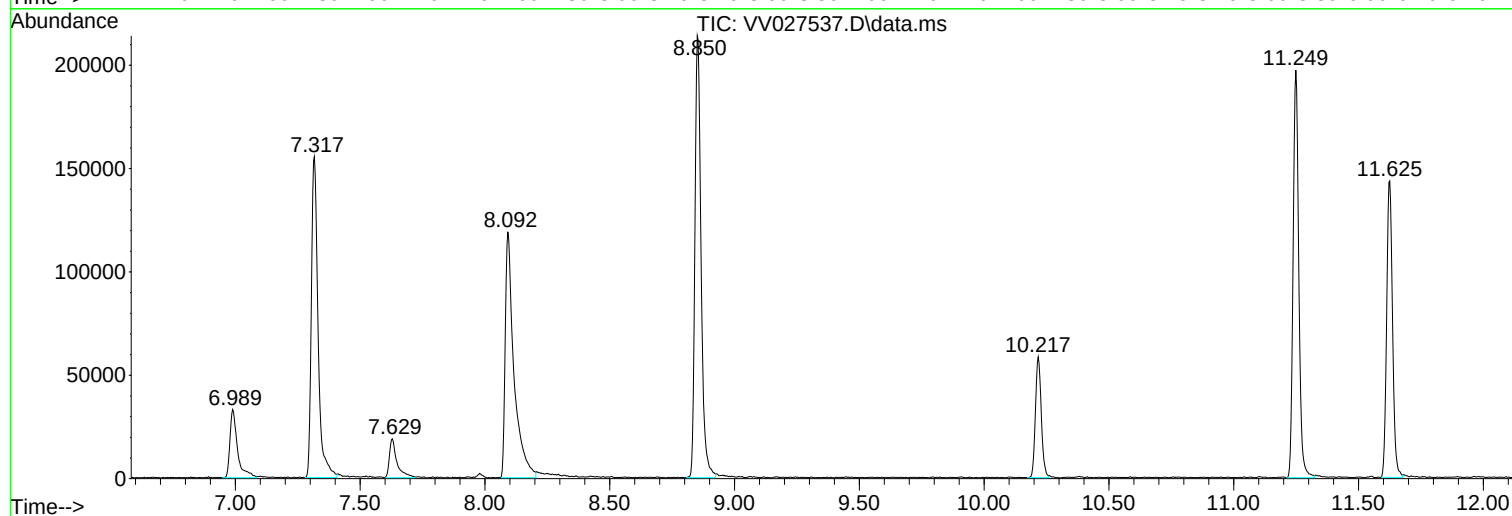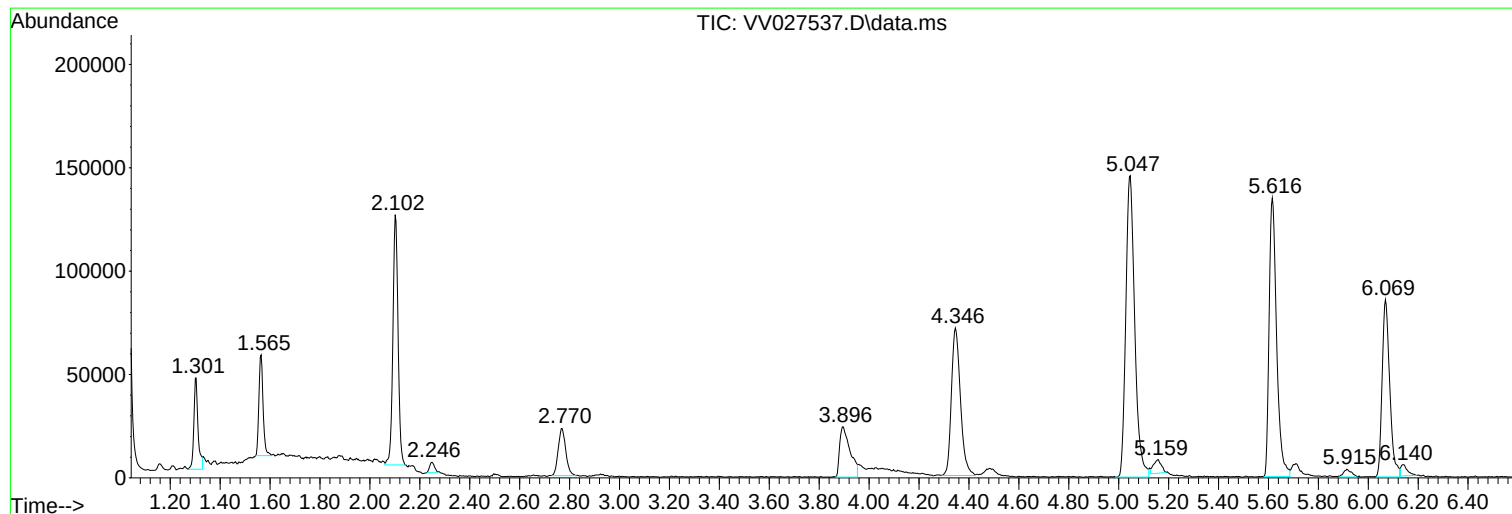

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027537.D
Acq On : 26 Aug 2022 16:01
Operator : SY/MD
Sample : N4368-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027537.D
Acq On : 26 Aug 2022 16:01
Operator : SY/MD
Sample : N4368-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5E96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc