

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027541.D
 Acq On : 26 Aug 2022 18:05
 Operator : SY/MD
 Sample : N4368-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	94	rBV	46083	55092	14.75%	1.740%
2	1.564	156	163	174	rBV	50359	58080	15.55%	1.835%
3	2.105	321	331	345	rVV	120411	176153	47.16%	5.564%
4	2.179	348	354	373	rVB6	6901	18429	4.93%	0.582%
5	3.902	879	890	909	rBV2	21979	69808	18.69%	2.205%
6	4.346	1013	1028	1049	rBV	68022	176283	47.20%	5.568%
7	5.047	1231	1246	1279	rBV2	141391	373496	100.00%	11.798%
8	5.616	1412	1423	1457	rBV	139947	304225	81.45%	9.610%
9	5.918	1506	1517	1538	rBV5	16346	37552	10.05%	1.186%
10	6.069	1551	1564	1592	rBV2	85023	186771	50.01%	5.900%
11	6.992	1840	1851	1866	rBV	31942	64449	17.26%	2.036%
12	7.317	1941	1952	1974	rBV	153692	285796	76.52%	9.028%
13	7.628	2037	2049	2064	rBV2	17225	34948	9.36%	1.104%
14	7.979	2148	2158	2175	rVB5	14301	25819	6.91%	0.816%
15	8.091	2183	2193	2232	rBV	112117	279434	74.82%	8.827%
16	8.850	2419	2429	2457	rBV	219074	372453	99.72%	11.765%
17	10.214	2842	2853	2869	rBV	55994	90536	24.24%	2.860%
18	11.249	3164	3175	3195	rBV	202651	316159	84.65%	9.987%
19	11.622	3279	3291	3308	rBV	144558	235119	62.95%	7.427%
20	16.178	4701	4708	4714	rBV8	4894	5198	1.39%	0.164%




Sum of corrected areas: 3165800

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027541.D
Acq On : 26 Aug 2022 18:05
Operator : SY/MD
Sample : N4368-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

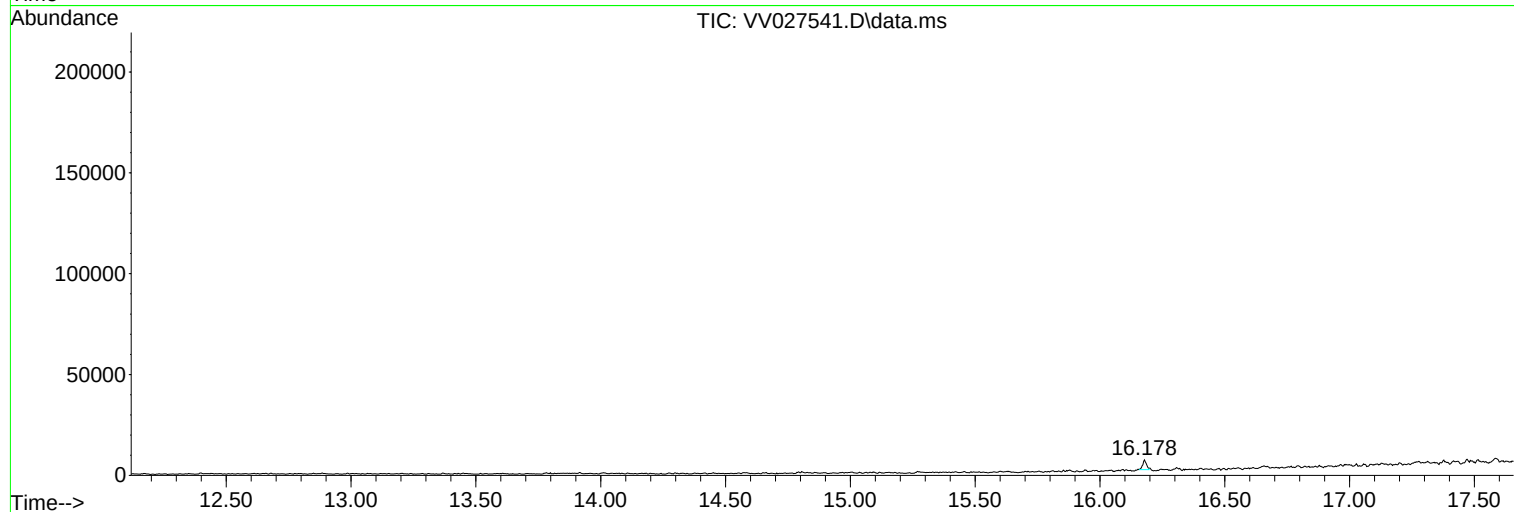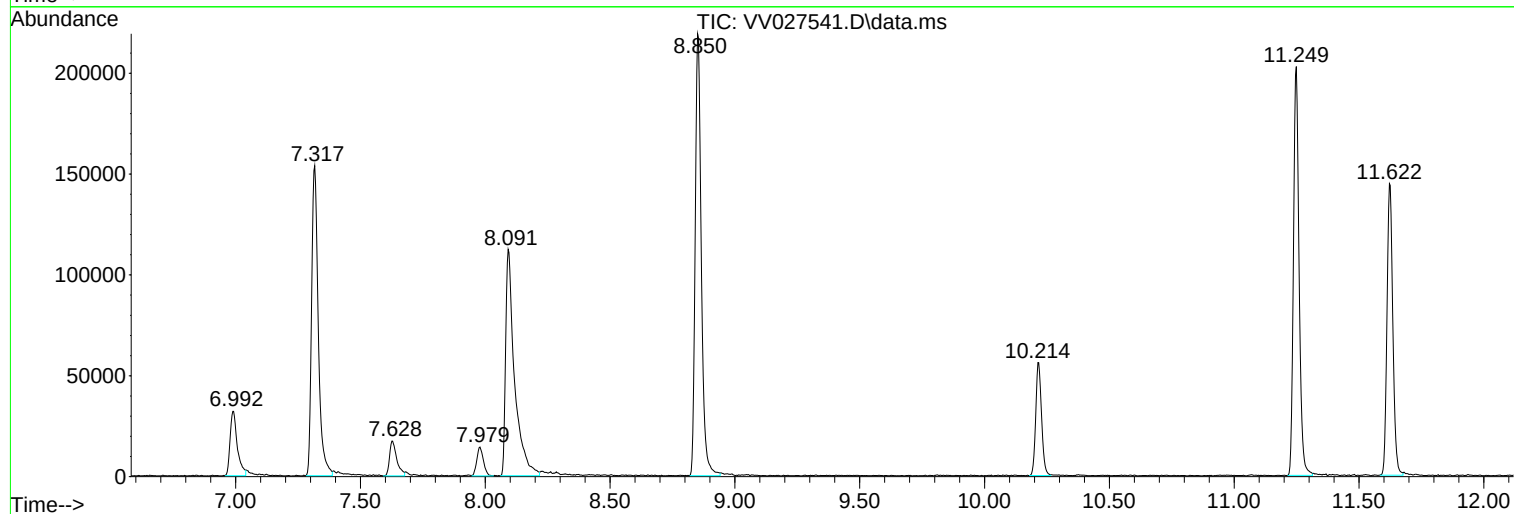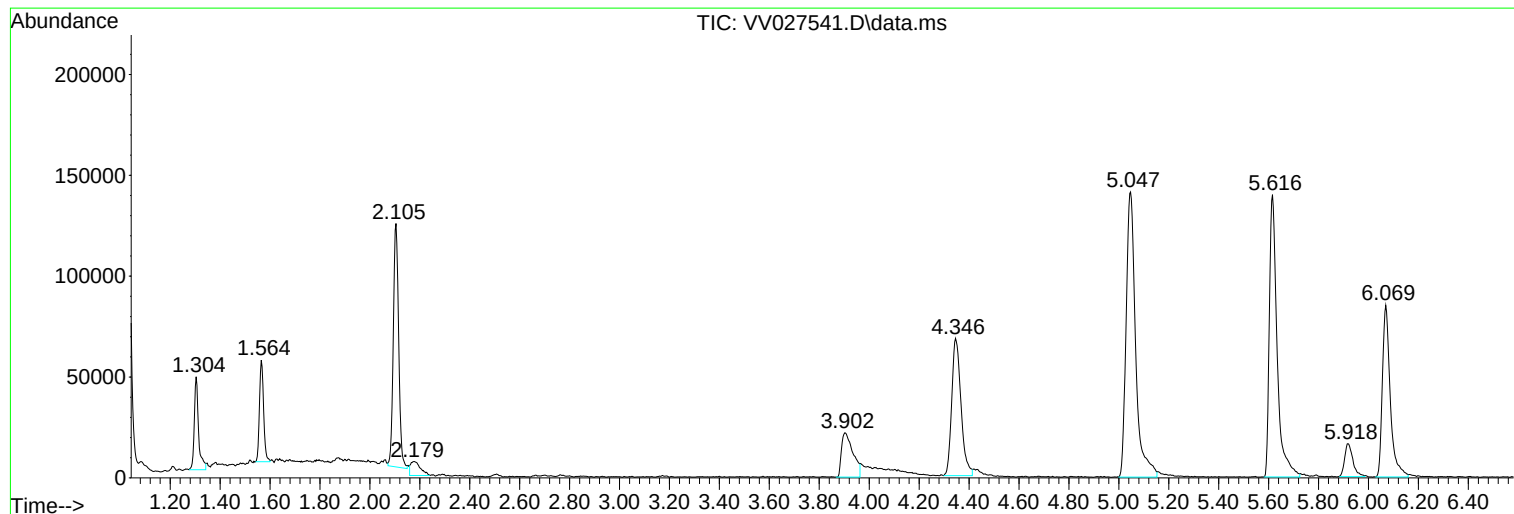

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027541.D
Acq On : 26 Aug 2022 18:05
Operator : SY/MD
Sample : N4368-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
Data File : VV027541.D
Acq On : 26 Aug 2022 18:05
Operator : SY/MD
Sample : N4368-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc