
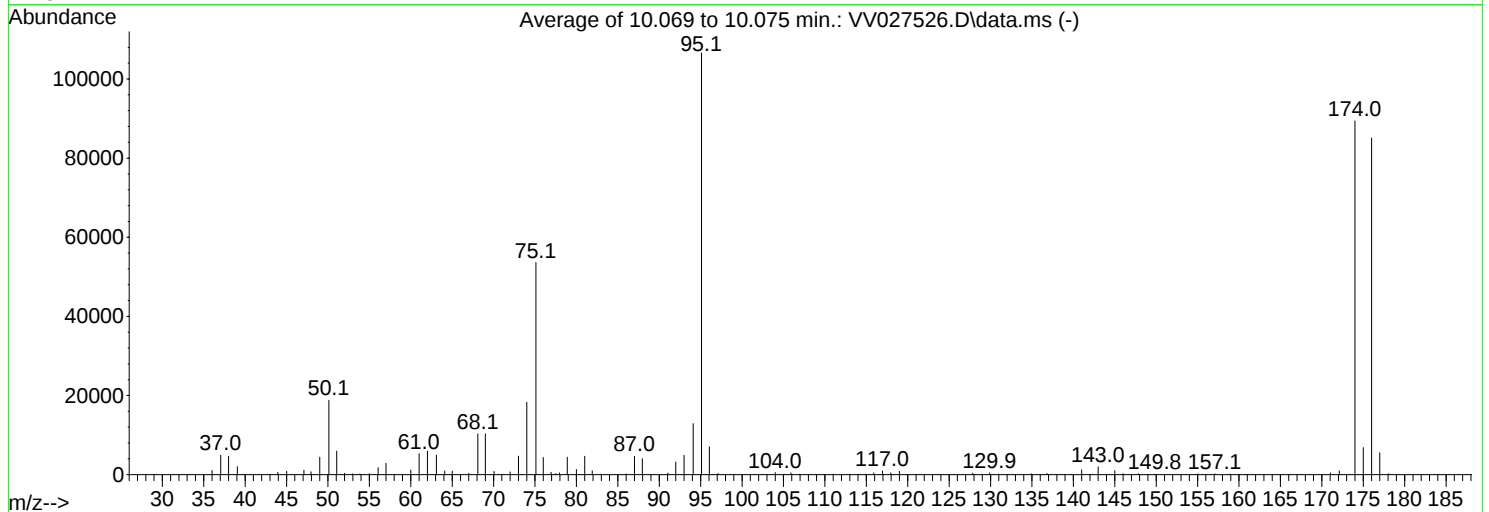


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082622\
 Data File : VV027526.D
 Acq On : 26 Aug 2022 08:52
 Operator : SY/MD
 Sample : BFB361
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB361

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 27 03:12:26 2022

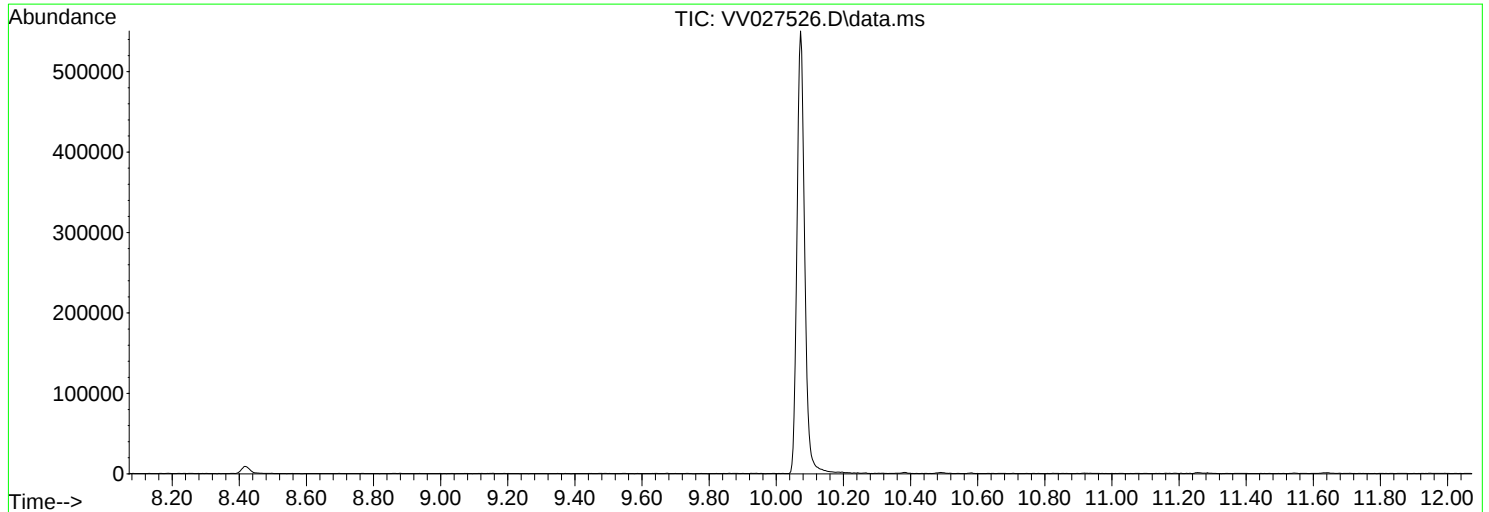

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	18768	PASS
75	95	30	80	50.3	53624	PASS
95	95	100	100	100.0	106613	PASS
96	95	5	9	6.6	7030	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.8	89371	PASS
175	174	5	9	7.6	6825	PASS
176	174	95	105	95.2	85107	PASS
177	176	5	10	6.5	5560	PASS

m/z	Abundance
39.90	159.0
44.00	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361

m/z	Abundance
36.00	994.0
37.00	4889.0
38.00	4383.0
39.10	2015.0
40.00	278.0
44.00	835.0
45.00	833.0
46.20	135.0
47.10	1020.0
48.00	664.0
49.00	4452.0
50.10	18400.0
51.00	6317.0
52.00	328.0
52.90	260.0
53.80	151.0
54.90	313.0
56.00	1792.0
57.00	2853.0
58.00	126.0
60.00	1095.0
61.00	5141.0
62.00	5821.0
63.10	4859.0
64.10	982.0
65.00	784.0
65.90	129.0
67.00	276.0
68.10	9843.0
69.00	9924.0
70.00	741.0
72.00	686.0
73.00	4500.0
74.00	18056.0
75.10	53296.0
76.00	4454.0
76.90	569.0
77.50	398.0
78.00	408.0
78.90	4387.0
80.00	1290.0
81.00	4551.0
81.90	845.0
82.90	118.0
86.00	259.0
87.00	4491.0
88.00	4105.0
91.00	457.0
92.00	3119.0
93.00	4644.0
94.10	12763.0
95.10	104920.0
96.00	7024.0
97.10	277.0
104.00	467.0
105.10	175.0
105.90	444.0
106.80	101.0
108.00	114.0
109.90	119.0
111.00	125.0
113.10	102.0
114.90	173.0
115.90	426.0
117.00	942.0
117.90	365.0
119.00	803.0
127.80	381.0
129.10	121.0
129.80	466.0
130.90	168.0
134.90	248.0
136.80	245.0
139.80	107.0
141.00	1118.0
141.90	148.0
143.00	1879.0
145.00	1039.0
146.00	242.0
147.80	283.0
148.80	124.0
149.90	127.0
154.80	264.0
157.10	205.0
158.90	122.0
171.10	447.0
172.10	978.0
174.00	85256.0
175.00	6633.0
176.00	81912.0
177.00	5498.0
178.10	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361

m/z	Abundance
36.00	1117.0
37.10	5069.0
38.00	4815.0
39.10	2075.0
40.00	263.0
43.90	832.0
45.00	899.0
45.90	109.0
47.10	1138.0
47.90	743.0
49.00	4579.0
50.10	19488.0
51.00	6138.0
52.00	357.0
52.90	218.0
53.90	181.0
55.00	285.0
56.10	1864.0
57.00	2918.0
58.20	144.0
60.00	1227.0
61.00	5543.0
62.00	6113.0
63.10	5127.0
64.10	977.0
65.00	886.0
66.00	106.0
67.00	354.0
68.10	10764.0
69.00	10623.0
70.00	825.0
72.00	746.0
73.00	4892.0
74.00	18976.0
75.10	55536.0
76.00	4398.0
77.00	610.0
77.50	387.0
77.90	467.0
78.90	4565.0
80.00	1347.0
81.00	4833.0
81.90	1006.0
83.00	132.0
86.00	222.0
87.00	4836.0
88.00	4249.0
91.00	426.0
92.00	3265.0
93.00	5065.0
94.10	13364.0
95.10	110448.0
96.10	7263.0
97.10	303.0
104.00	556.0
105.00	180.0
105.90	469.0
106.90	103.0
109.90	101.0
111.00	137.0
113.00	114.0
115.00	194.0
115.90	448.0
117.00	955.0
117.90	466.0
119.00	888.0
119.80	119.0
127.90	347.0
128.90	120.0
129.90	462.0
131.00	144.0
134.90	272.0
136.80	280.0
138.90	111.0
139.80	116.0
141.00	1269.0
143.00	2075.0
145.00	1053.0
146.00	256.0
147.80	246.0
149.90	137.0
155.00	274.0
157.10	223.0
158.90	145.0
160.70	104.0
171.00	438.0
172.10	1026.0
174.00	92488.0
175.00	7065.0
176.00	88056.0
177.00	5737.0
178.10	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361

m/z	Abundance
36.00	1019.0
37.10	4696.0
38.00	4641.0
39.00	1964.0
40.00	272.0
43.90	859.0
45.00	873.0
45.90	119.0
47.10	1201.0
47.90	797.0
49.00	4148.0
50.10	18416.0
51.10	5445.0
52.00	340.0
53.00	160.0
53.90	193.0
55.10	242.0
56.10	1676.0
57.00	2867.0
58.20	148.0
60.00	1236.0
61.00	5182.0
62.00	5872.0
63.10	4769.0
64.10	895.0
65.00	947.0
67.00	379.0
68.10	10315.0
69.00	10414.0
70.10	818.0
72.00	663.0
73.00	4699.0
74.00	17896.0
75.10	52040.0
76.00	4099.0
77.00	614.0
77.90	500.0
78.90	4295.0
80.00	1283.0
81.00	4536.0
81.90	1082.0
83.00	152.0
86.00	165.0
87.00	4508.0
87.90	3827.0
91.10	386.0
92.00	3153.0
93.00	5009.0
94.10	12632.0
95.10	104472.0
96.10	6804.0
97.10	277.0
104.00	584.0
105.00	183.0
105.90	461.0
107.00	116.0
111.00	131.0
112.00	112.0
112.90	109.0
115.00	171.0
115.90	436.0
116.90	885.0
118.00	513.0
119.00	889.0
119.80	105.0
127.90	326.0
128.90	155.0
130.00	453.0
131.00	157.0
134.90	255.0
136.80	289.0
138.90	134.0
141.00	1304.0
143.00	1965.0
145.00	968.0
146.00	231.0
147.90	193.0
149.80	137.0
155.10	317.0
157.10	225.0
158.90	177.0
171.00	406.0
172.10	931.0
174.00	90368.0
175.00	6777.0
176.00	85352.0
177.00	5444.0
178.10	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB361