

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037039.D
 Acq On : 26 Aug 2024 19:35
 Operator : SY/MD
 Sample : P3692-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA6

Quant Time: Aug 27 02:05:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 27 01:58:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	622164	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	589245	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	283954	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	244593	42.977	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	85.960%	
7) Chloroethane-d5	1.529	69	204915	46.587	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	93.180%	
11) 1,1-Dichloroethene-d2	2.056	65	109861	45.927	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.860%	
21) 2-Butanone-d5	3.796	46	266751	121.033	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	121.030%	
24) Chloroform-d	4.243	84	426944	47.931	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.860%	
26) 1,2-Dichloroethane-d4	4.937	65	285341	50.868	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.740%	
32) Benzene-d6	4.953	84	900458	50.595	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.180%	
36) 1,2-Dichloropropane-d6	5.986	67	293450	52.642	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	105.280%	
41) Toluene-d8	7.240	98	798895	49.737	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.480%	
43) trans-1,3-Dichloroprop...	7.551	79	125780	48.771	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.540%	
47) 2-Hexanone-d5	8.024	63	179493	117.982	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	117.980%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	361928	53.534	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	107.060%	
66) 1,2-Dichlorobenzene-d4	11.554	152	292187	51.378	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.760%	
Target Compounds						
13) Acetone	2.114	43	11610	4.912	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037039.D
Acq On : 26 Aug 2024 19:35
Operator : SY/MD
Sample : P3692-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA6

Quant Time: Aug 27 02:05:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 27 01:58:15 2024
Response via : Initial Calibration

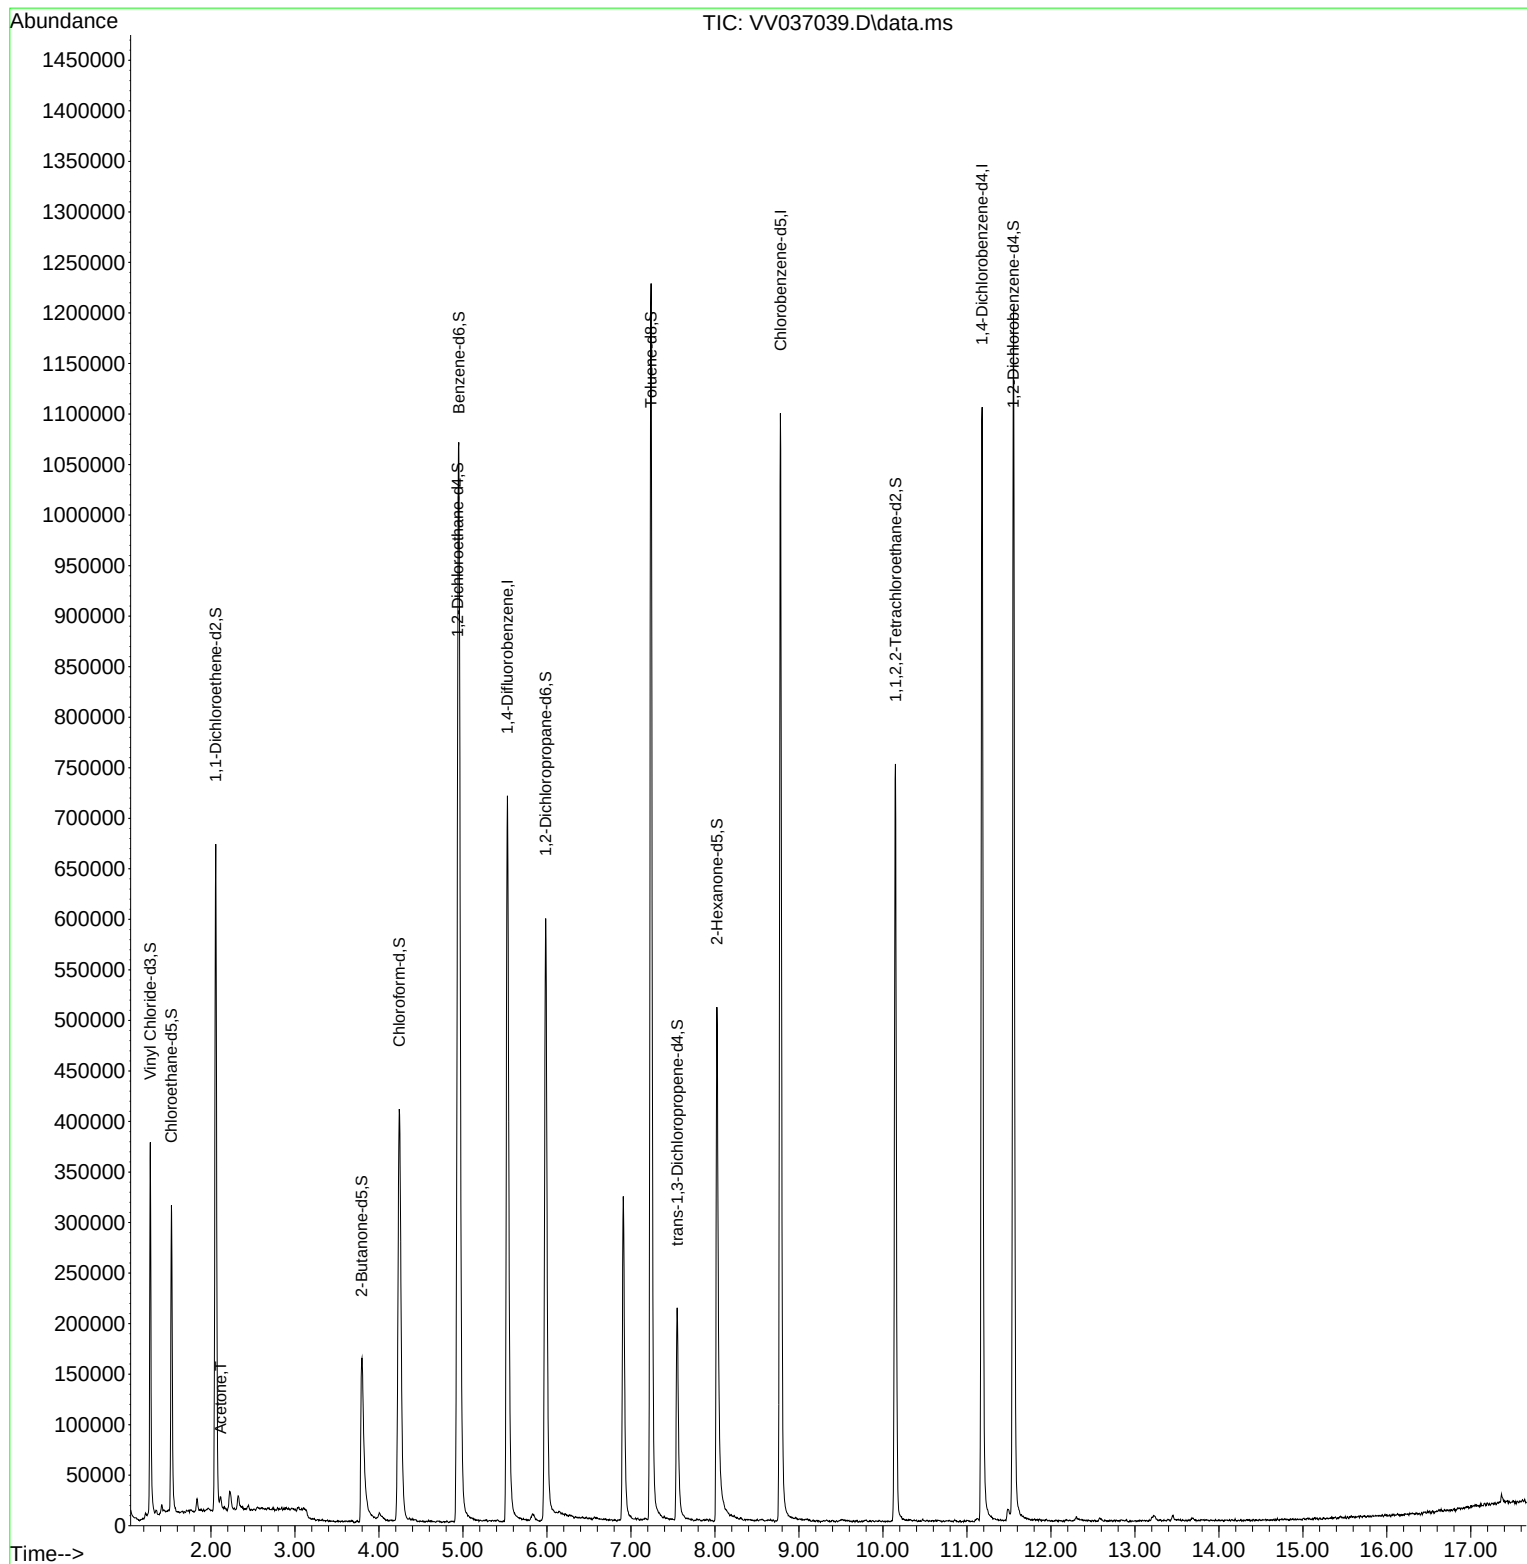

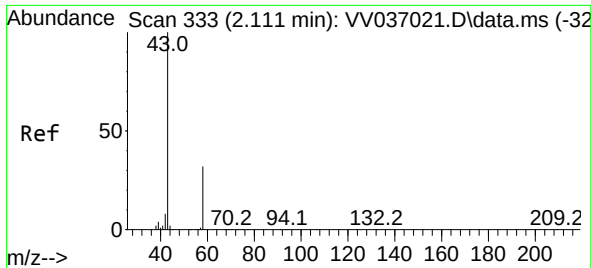

#13
 Acetone
 Concen: 4.912 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV037039.D
 Acq: 26 Aug 2024 19:35

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA6

Tgt Ion: 43 Resp: 11610
 Ion Ratio Lower Upper
 43 100
 58 34.2 0.0 64.8

