

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037043.D
 Acq On : 26 Aug 2024 21:03
 Operator : SY/MD
 Sample : P3693-17
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K91

Quant Time: Aug 27 02:06:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 27 01:58:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	598435	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	574220	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	271713	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	230621	42.128	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.260%
7) Chloroethane-d5	1.529	69	197825	46.758	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.520%
11) 1,1-Dichloroethene-d2	2.056	65	104362	45.358	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.720%
21) 2-Butanone-d5	3.796	46	242761	114.515	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	114.520%
24) Chloroform-d	4.243	84	411160	47.990	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.980%
26) 1,2-Dichloroethane-d4	4.937	65	275925	51.140	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.280%
32) Benzene-d6	4.953	84	864438	49.842	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.680%
36) 1,2-Dichloropropane-d6	5.985	67	281125	51.751	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.500%
41) Toluene-d8	7.239	98	774762	49.497	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	7.551	79	115621	46.005	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.020%
47) 2-Hexanone-d5	8.024	63	161540	108.960	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.960%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	340495	51.682	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.360%
66) 1,2-Dichlorobenzene-d4	11.558	152	279595	51.378	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.760%
Target Compounds						
13) Acetone	2.114	43	9324	4.101	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037043.D
Acq On : 26 Aug 2024 21:03
Operator : SY/MD
Sample : P3693-17
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K91

Quant Time: Aug 27 02:06:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 27 01:58:15 2024
Response via : Initial Calibration

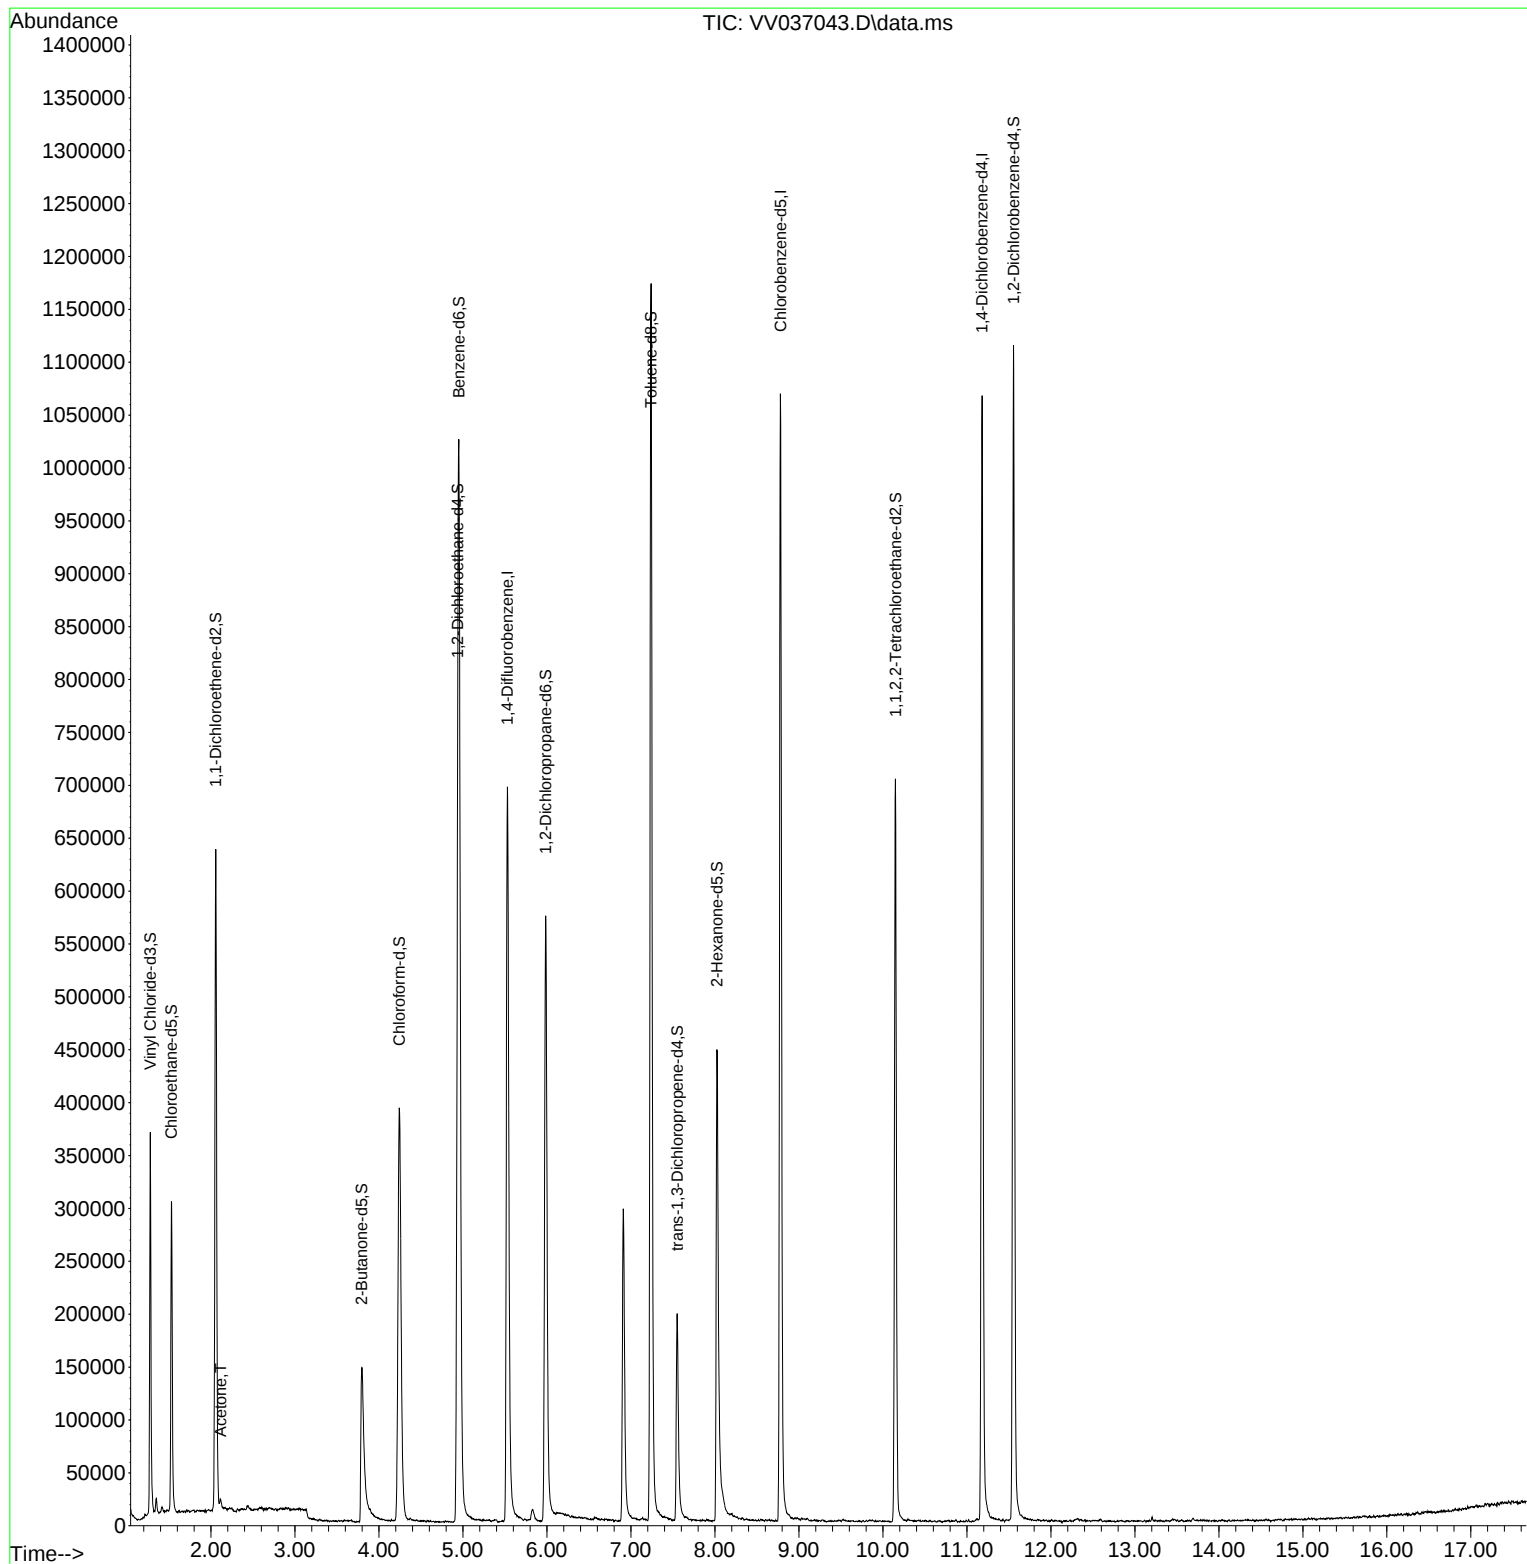

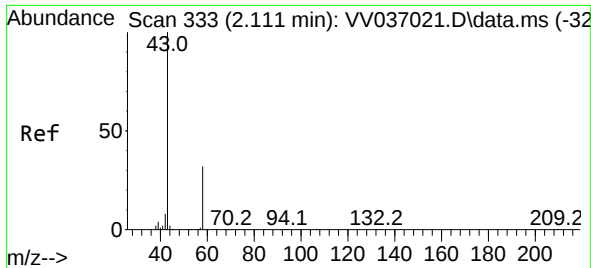

#13
 Acetone
 Concen: 4.101 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV037043.D
 Acq: 26 Aug 2024 21:03

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K91

Tgt Ion: 43 Resp: 9324
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 64.8

