

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037023.D
 Acq On : 26 Aug 2024 13:40
 Operator : SY/MD
 Sample : VV0826WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	433338	461554	16.86%	2.291%
2	1.532	146	153	164	rBV	333760	388888	14.21%	1.930%
3	2.059	308	317	332	rVB	699477	1001613	36.59%	4.971%
4	3.468	751	755	759	rBV6	1333	1273	0.05%	0.006%
5	3.510	766	768	771	rBV4	1053	588	0.02%	0.003%
6	3.664	812	816	819	rBV4	1129	899	0.03%	0.004%
7	3.703	824	828	830	rVB4	1038	699	0.03%	0.003%
8	3.799	849	858	895	rBV	145148	417402	15.25%	2.072%
9	4.243	982	996	1024	rBV	412004	1067253	38.99%	5.297%
10	4.645	1119	1121	1123	rBV3	858	614	0.02%	0.003%
11	4.770	1156	1160	1162	rBV3	1957	1441	0.05%	0.007%
12	4.844	1179	1183	1186	rBV4	899	686	0.03%	0.003%
13	4.863	1186	1189	1191	rVB3	751	427	0.02%	0.002%
14	4.876	1191	1193	1194	rBV2	950	490	0.02%	0.002%
15	4.950	1200	1216	1242	rBV2	1091839	2737344	100.00%	13.586%
16	5.452	1371	1372	1376	rVB4	1944	986	0.04%	0.005%
17	5.477	1376	1380	1381	rBV4	1270	944	0.03%	0.005%
18	5.529	1385	1396	1427	rBV	762539	1564263	57.15%	7.764%
19	5.828	1480	1489	1509	rBV	11066	26925	0.98%	0.134%
20	5.985	1526	1538	1564	rBV	601831	1234566	45.10%	6.127%
21	6.458	1681	1685	1686	rBV4	1515	1112	0.04%	0.006%
22	6.532	1703	1708	1711	rBV5	973	891	0.03%	0.004%
23	6.574	1717	1721	1722	rBV3	891	549	0.02%	0.003%
24	6.638	1739	1741	1744	rBV4	1432	844	0.03%	0.004%
25	6.667	1744	1750	1753	rBV5	1491	1513	0.06%	0.008%
26	6.693	1753	1758	1760	rBV5	1482	1231	0.04%	0.006%
27	6.722	1765	1767	1768	rVB2	1141	323	0.01%	0.002%
28	6.763	1778	1780	1784	rVB4	1082	725	0.03%	0.004%
29	6.783	1784	1786	1787	rBV2	1057	443	0.02%	0.002%
30	6.802	1789	1792	1795	rBV6	744	594	0.02%	0.003%
31	6.911	1815	1826	1852	rBV	318433	613920	22.43%	3.047%
32	7.239	1917	1928	1967	rBV	1246851	2199360	80.35%	10.916%
33	7.477	2000	2002	2007	rBV5	1717	1300	0.05%	0.006%
34	7.551	2016	2025	2058	rBV2	206988	385876	14.10%	1.915%
35	8.027	2164	2173	2208	rBV2	450809	957443	34.98%	4.752%
36	8.677	2369	2375	2377	rBV5	1601	1704	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037023.D
 Acq On : 26 Aug 2024 13:40
 Operator : SY/MD
 Sample : VV0826WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.779	2396	2407	2436	rBV	1178593	1938213	70.81%	9.620%
38	9.278	2560	2562	2565	rBV2	928	695	0.03%	0.003%
39	9.320	2573	2575	2576	rBV2	1446	509	0.02%	0.003%
40	9.352	2579	2585	2586	rBV5	1421	1243	0.05%	0.006%
41	9.480	2619	2625	2631	rBV10	3238	5803	0.21%	0.029%
42	9.619	2665	2668	2669	rBV3	1661	893	0.03%	0.004%
43	9.722	2697	2700	2703	rBV4	1422	1216	0.04%	0.006%
44	9.779	2714	2718	2720	rBV5	1721	1219	0.04%	0.006%
45	9.812	2726	2728	2733	rVB6	1867	907	0.03%	0.005%
46	9.866	2740	2745	2749	rBV7	3167	3574	0.13%	0.018%
47	9.950	2768	2771	2772	rBV2	1399	769	0.03%	0.004%
48	9.988	2781	2783	2785	rVB2	831	268	0.01%	0.001%
49	10.027	2790	2795	2798	rBV7	1450	1088	0.04%	0.005%
50	10.149	2821	2833	2864	rBV	721044	1150520	42.03%	5.710%
51	10.442	2919	2924	2926	rBV6	888	732	0.03%	0.004%
52	10.458	2927	2929	2931	rBV3	841	493	0.02%	0.002%
53	10.599	2971	2973	2974	rBV2	707	214	0.01%	0.001%
54	10.644	2985	2987	2988	rBV2	940	286	0.01%	0.001%
55	10.680	2996	2998	2999	rBV	936	386	0.01%	0.002%
56	10.715	3008	3009	3013	rBV3	609	403	0.01%	0.002%
57	10.750	3013	3020	3023	rVB7	1448	1703	0.06%	0.008%
58	10.776	3023	3028	3029	rBV4	1454	1163	0.04%	0.006%
59	10.824	3041	3043	3044	rBV2	1092	544	0.02%	0.003%
60	10.850	3047	3051	3052	rBV4	2847	2124	0.08%	0.011%
61	10.911	3067	3070	3071	rBV3	997	530	0.02%	0.003%
62	10.943	3077	3080	3083	rBV4	1427	1172	0.04%	0.006%
63	10.959	3083	3085	3086	rBV2	827	338	0.01%	0.002%
64	11.001	3093	3098	3100	rBV4	1431	1218	0.04%	0.006%
65	11.021	3100	3104	3106	rBV4	662	539	0.02%	0.003%
66	11.075	3119	3121	3124	rVB4	1127	545	0.02%	0.003%
67	11.123	3130	3136	3139	rBV8	6814	7967	0.29%	0.040%
68	11.181	3143	3154	3186	rVV	1194149	1908588	69.72%	9.473%
69	11.554	3259	3270	3302	rBV	1201174	1926792	70.39%	9.563%
70	11.860	3358	3365	3367	rBV8	2411	2981	0.11%	0.015%
71	11.908	3373	3380	3384	rBV7	1940	2299	0.08%	0.011%
72	12.024	3413	3416	3418	rBV4	1320	945	0.03%	0.005%
73	12.168	3457	3461	3462	rBV4	1780	1113	0.04%	0.006%
74	12.371	3521	3524	3528	rBV4	1453	1361	0.05%	0.007%
75	12.458	3549	3551	3555	rVB3	1001	471	0.02%	0.002%
76	12.683	3619	3621	3624	rBV3	1065	720	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037023.D
 Acq On : 26 Aug 2024 13:40
 Operator : SY/MD
 Sample : VV0826WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.728	3632	3635	3637	rBV3	1041	548	0.02%	0.003%
78	12.811	3658	3661	3662	rBV3	1509	859	0.03%	0.004%
79	12.885	3679	3684	3687	rBV4	1623	1509	0.06%	0.007%
80	12.988	3712	3716	3723	rBV7	1857	2494	0.09%	0.012%
81	13.037	3727	3731	3732	rBV3	887	626	0.02%	0.003%
82	13.207	3776	3784	3792	rBV6	10451	18413	0.67%	0.091%
83	13.397	3841	3843	3847	rVB3	1928	842	0.03%	0.004%
84	13.445	3847	3858	3871	rBV2	23235	49113	1.79%	0.244%
85	13.606	3905	3908	3913	rBV6	1578	1106	0.04%	0.005%
86	13.683	3924	3932	3945	rBV9	10741	20247	0.74%	0.100%
87	14.249	4105	4108	4112	rBV4	1562	1194	0.04%	0.006%
88	14.287	4115	4120	4125	rBV9	1620	2477	0.09%	0.012%




Sum of corrected areas: 20148655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037023.D
Acq On : 26 Aug 2024 13:40
Operator : SY/MD
Sample : VV0826WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

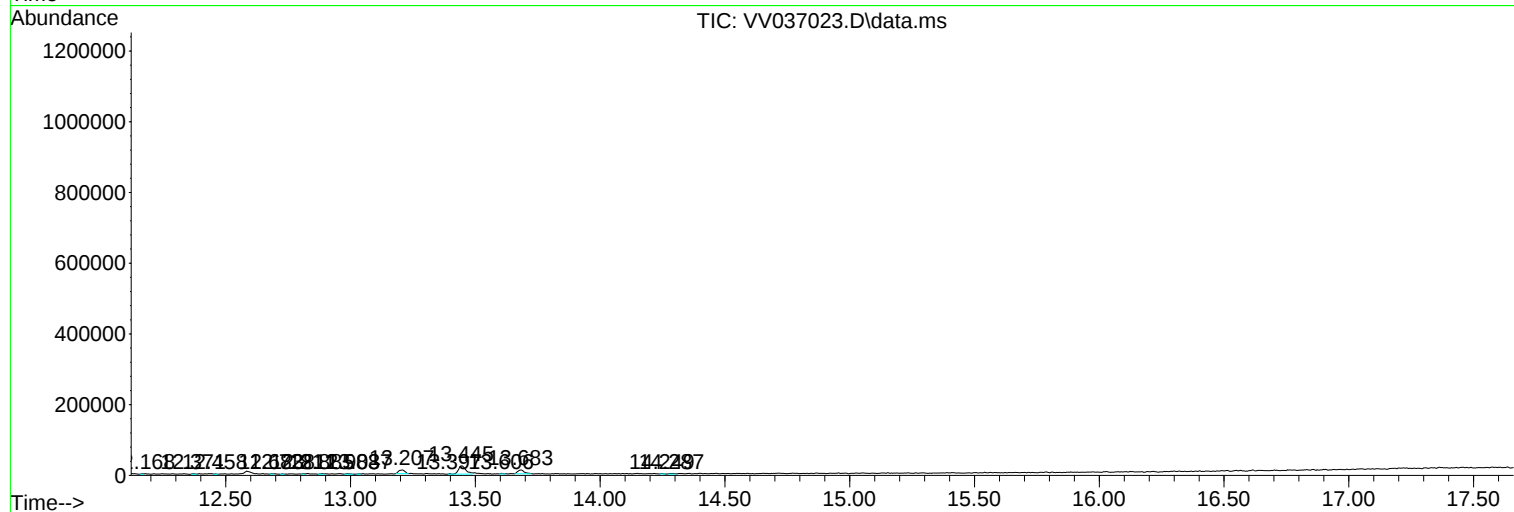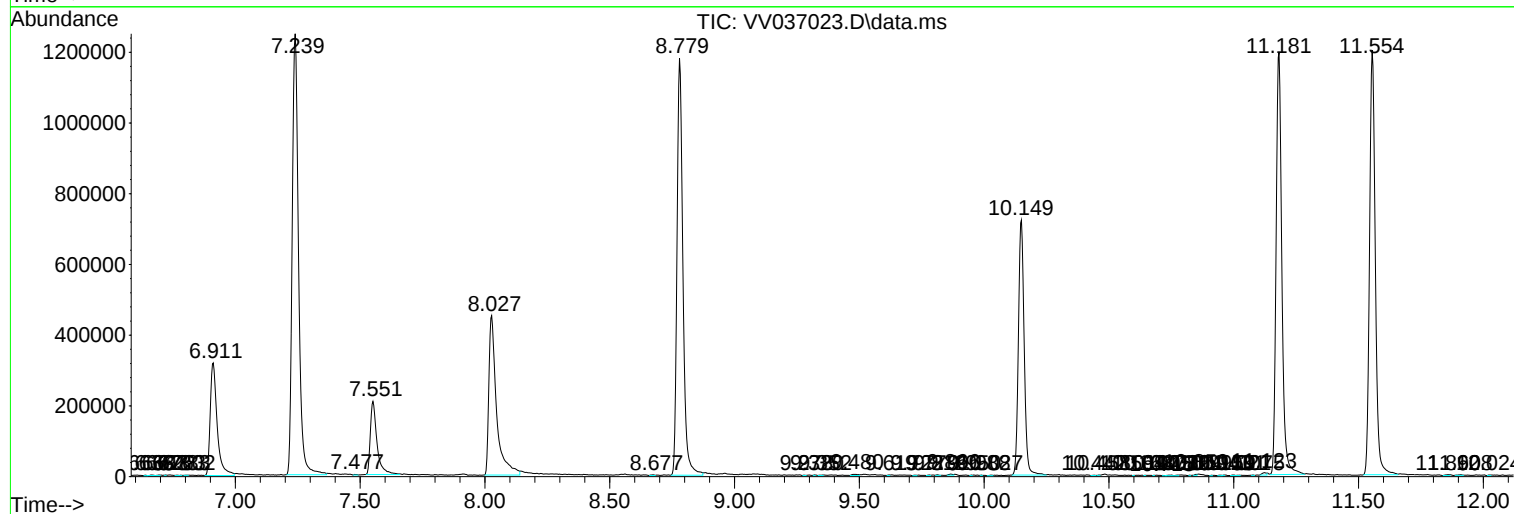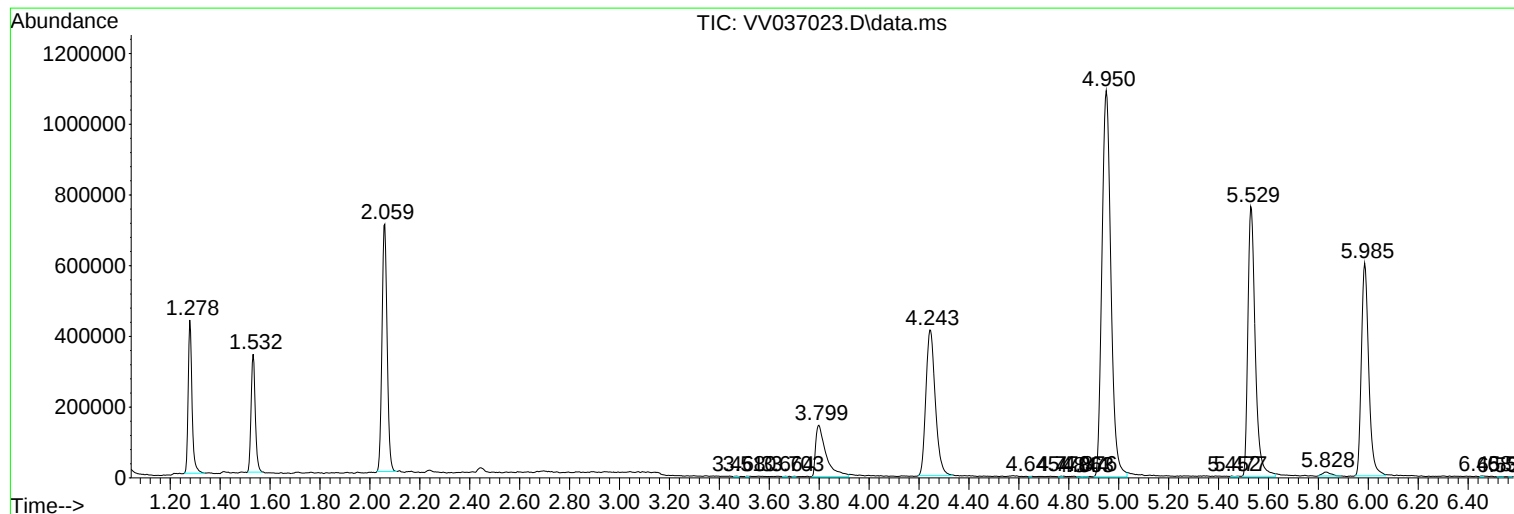

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037023.D
Acq On : 26 Aug 2024 13:40
Operator : SY/MD
Sample : VV0826WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037023.D
Acq On : 26 Aug 2024 13:40
Operator : SY/MD
Sample : VV0826WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
