

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037037.D
 Acq On : 26 Aug 2024 18:51
 Operator : SY/MD
 Sample : P3692-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	35	39	40	rBV3	1120	869	0.03%	0.004%
2	1.278	67	74	90	rVB	371577	388844	14.69%	1.999%
3	1.413	112	116	124	rBV7	7136	11223	0.42%	0.058%
4	1.532	145	153	166	rVB	299915	360449	13.62%	1.853%
5	2.057	306	316	330	rBV	645786	925877	34.98%	4.760%
6	3.497	762	764	769	rVB5	1375	1081	0.04%	0.006%
7	3.558	779	783	786	rBV6	1173	979	0.04%	0.005%
8	3.796	848	857	891	rBV	162145	445893	16.85%	2.292%
9	4.066	939	941	944	rBV4	1848	1286	0.05%	0.007%
10	4.143	962	965	970	rVB6	1417	1115	0.04%	0.006%
11	4.182	974	977	978	rBV3	1624	882	0.03%	0.005%
12	4.243	980	996	1027	rVV2	401361	1040554	39.32%	5.349%
13	4.613	1110	1111	1119	rVB6	1159	1109	0.04%	0.006%
14	4.654	1119	1124	1125	rBV4	1302	1084	0.04%	0.006%
15	4.661	1125	1126	1132	rVB5	1025	797	0.03%	0.004%
16	4.706	1136	1140	1142	rBV5	1142	850	0.03%	0.004%
17	4.793	1163	1167	1170	rVB5	1099	738	0.03%	0.004%
18	4.950	1200	1216	1253	rBV2	1056154	2646578	100.00%	13.606%
19	5.230	1299	1303	1305	rVB4	1143	797	0.03%	0.004%
20	5.529	1385	1396	1428	rBV	733106	1503974	56.83%	7.732%
21	5.783	1472	1475	1478	rBV4	1285	1147	0.04%	0.006%
22	5.825	1478	1488	1496	rBV10	8776	17911	0.68%	0.092%
23	5.986	1524	1538	1567	rBV	583447	1232100	46.55%	6.334%
24	6.780	1783	1785	1790	rBV5	1205	1002	0.04%	0.005%
25	6.908	1813	1825	1850	rBV	316789	596371	22.53%	3.066%
26	7.240	1916	1928	1948	rBV	1203449	2106551	79.60%	10.829%
27	7.551	2014	2025	2048	rVV	205073	379380	14.33%	1.950%
28	7.783	2094	2097	2102	rBV6	1925	1503	0.06%	0.008%
29	7.876	2123	2126	2131	rVB6	944	875	0.03%	0.004%
30	7.899	2131	2133	2135	rBV2	2046	1208	0.05%	0.006%
31	7.960	2148	2152	2155	rBV5	1450	1239	0.05%	0.006%
32	8.024	2163	2172	2205	rBV	494249	968148	36.58%	4.977%
33	8.468	2306	2310	2314	rBV6	1474	1388	0.05%	0.007%
34	8.545	2330	2334	2336	rBV4	1247	1032	0.04%	0.005%
35	8.603	2350	2352	2358	rVB5	1159	788	0.03%	0.004%
36	8.629	2358	2360	2365	rBV5	1008	848	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037037.D
 Acq On : 26 Aug 2024 18:51
 Operator : SY/MD
 Sample : P3692-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.780	2395	2407	2441	rBV	1125309	1857731	70.19%	9.550%
38	9.185	2528	2533	2535	rBV5	1452	1426	0.05%	0.007%
39	9.281	2561	2563	2565	rBV2	1365	730	0.03%	0.004%
40	9.362	2583	2588	2593	rBV7	1973	1733	0.07%	0.009%
41	9.423	2603	2607	2611	rVB5	1148	864	0.03%	0.004%
42	9.584	2653	2657	2660	rVB5	1322	1227	0.05%	0.006%
43	9.699	2691	2693	2700	rVB8	1852	1708	0.06%	0.009%
44	9.741	2700	2706	2707	rBV6	1534	1323	0.05%	0.007%
45	9.831	2730	2734	2738	rVB4	1641	1381	0.05%	0.007%
46	9.863	2738	2744	2746	rBV7	2111	2303	0.09%	0.012%
47	9.937	2764	2767	2769	rVB4	1333	724	0.03%	0.004%
48	9.985	2777	2782	2784	rBV6	1236	1027	0.04%	0.005%
49	10.146	2818	2832	2855	rBV	727292	1173594	44.34%	6.033%
50	10.391	2905	2908	2911	rBV5	1312	940	0.04%	0.005%
51	10.468	2928	2932	2933	rBV3	1287	905	0.03%	0.005%
52	10.677	2994	2997	3001	rVB5	1296	755	0.03%	0.004%
53	10.767	3021	3025	3026	rBV3	891	740	0.03%	0.004%
54	10.799	3034	3035	3039	rVB4	1547	824	0.03%	0.004%
55	10.834	3043	3046	3048	rBV4	1016	781	0.03%	0.004%
56	10.857	3048	3053	3057	rBV6	1778	2332	0.09%	0.012%
57	10.998	3092	3097	3099	rBV5	1022	835	0.03%	0.004%
58	11.059	3111	3116	3119	rBV5	1662	1396	0.05%	0.007%
59	11.079	3119	3122	3125	rBV4	1144	775	0.03%	0.004%
60	11.098	3125	3128	3130	rBV3	1209	988	0.04%	0.005%
61	11.130	3130	3138	3142	rBV10	3657	4735	0.18%	0.024%
62	11.182	3143	3154	3183	rBV	1151097	1821125	68.81%	9.362%
63	11.416	3224	3227	3231	rBV4	1015	1234	0.05%	0.006%
64	11.490	3246	3250	3251	rBV4	2124	1579	0.06%	0.008%
65	11.555	3259	3270	3297	rBV	1179381	1855809	70.12%	9.540%
66	11.873	3365	3369	3370	rBV5	1302	962	0.04%	0.005%
67	11.931	3385	3387	3392	rVV5	1462	905	0.03%	0.005%
68	12.066	3425	3429	3431	rVB4	1398	981	0.04%	0.005%
69	12.188	3465	3467	3473	rVB6	1037	1089	0.04%	0.006%
70	12.300	3498	3502	3503	rBV4	1346	755	0.03%	0.004%
71	12.394	3529	3531	3534	rVB4	1734	1013	0.04%	0.005%
72	12.455	3547	3550	3552	rVB4	1546	1039	0.04%	0.005%
73	12.580	3586	3589	3590	rBV3	2371	1537	0.06%	0.008%
74	12.648	3606	3610	3613	rVB4	1296	977	0.04%	0.005%
75	12.754	3640	3643	3646	rVB5	1438	934	0.04%	0.005%
76	12.915	3689	3693	3695	rBV3	1785	1164	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037037.D
 Acq On : 26 Aug 2024 18:51
 Operator : SY/MD
 Sample : P3692-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	12.963	3705	3708	3710	rBV4	1241	803	0.03%	0.004%
78	13.027	3727	3728	3733	rVV5	1319	946	0.04%	0.005%
79	13.053	3733	3736	3737	rVV2	1170	745	0.03%	0.004%
80	13.091	3741	3748	3749	rBV6	1611	1634	0.06%	0.008%
81	13.111	3749	3754	3756	rBV5	1191	1015	0.04%	0.005%
82	13.149	3764	3766	3771	rVB5	1417	818	0.03%	0.004%
83	13.201	3777	3782	3792	rBV5	4802	9090	0.34%	0.047%
84	13.288	3806	3809	3811	rBV4	1096	769	0.03%	0.004%
85	13.329	3820	3822	3828	rVB6	1754	1319	0.05%	0.007%
86	13.362	3828	3832	3837	rBV7	2081	1787	0.07%	0.009%
87	13.458	3852	3862	3867	rBV3	5509	9417	0.36%	0.048%
88	13.526	3877	3883	3884	rBV5	1270	1043	0.04%	0.005%
89	13.561	3890	3894	3895	rBV4	1555	1007	0.04%	0.005%
90	13.686	3924	3933	3938	rBV4	5631	9130	0.34%	0.047%
91	13.976	4018	4023	4024	rBV5	1028	727	0.03%	0.004%
92	14.127	4066	4070	4071	rBV3	1867	1197	0.05%	0.006%
93	14.233	4100	4103	4111	rBV8	1799	2157	0.08%	0.011%
94	14.516	4187	4191	4194	rBV5	1596	1175	0.04%	0.006%
95	14.532	4194	4196	4200	rVB4	1469	1105	0.04%	0.006%
96	14.712	4248	4252	4254	rBV5	1599	1022	0.04%	0.005%
97	14.808	4280	4282	4284	rBV3	1382	853	0.03%	0.004%
98	15.037	4349	4353	4355	rBV4	2879	2424	0.09%	0.012%
99	15.133	4380	4383	4385	rBV3	2004	1188	0.04%	0.006%
100	15.172	4393	4395	4398	rBV4	1659	1296	0.05%	0.007%


Sum of corrected areas: 19452017

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037037.D
Acq On : 26 Aug 2024 18:51
Operator : SY/MD
Sample : P3692-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

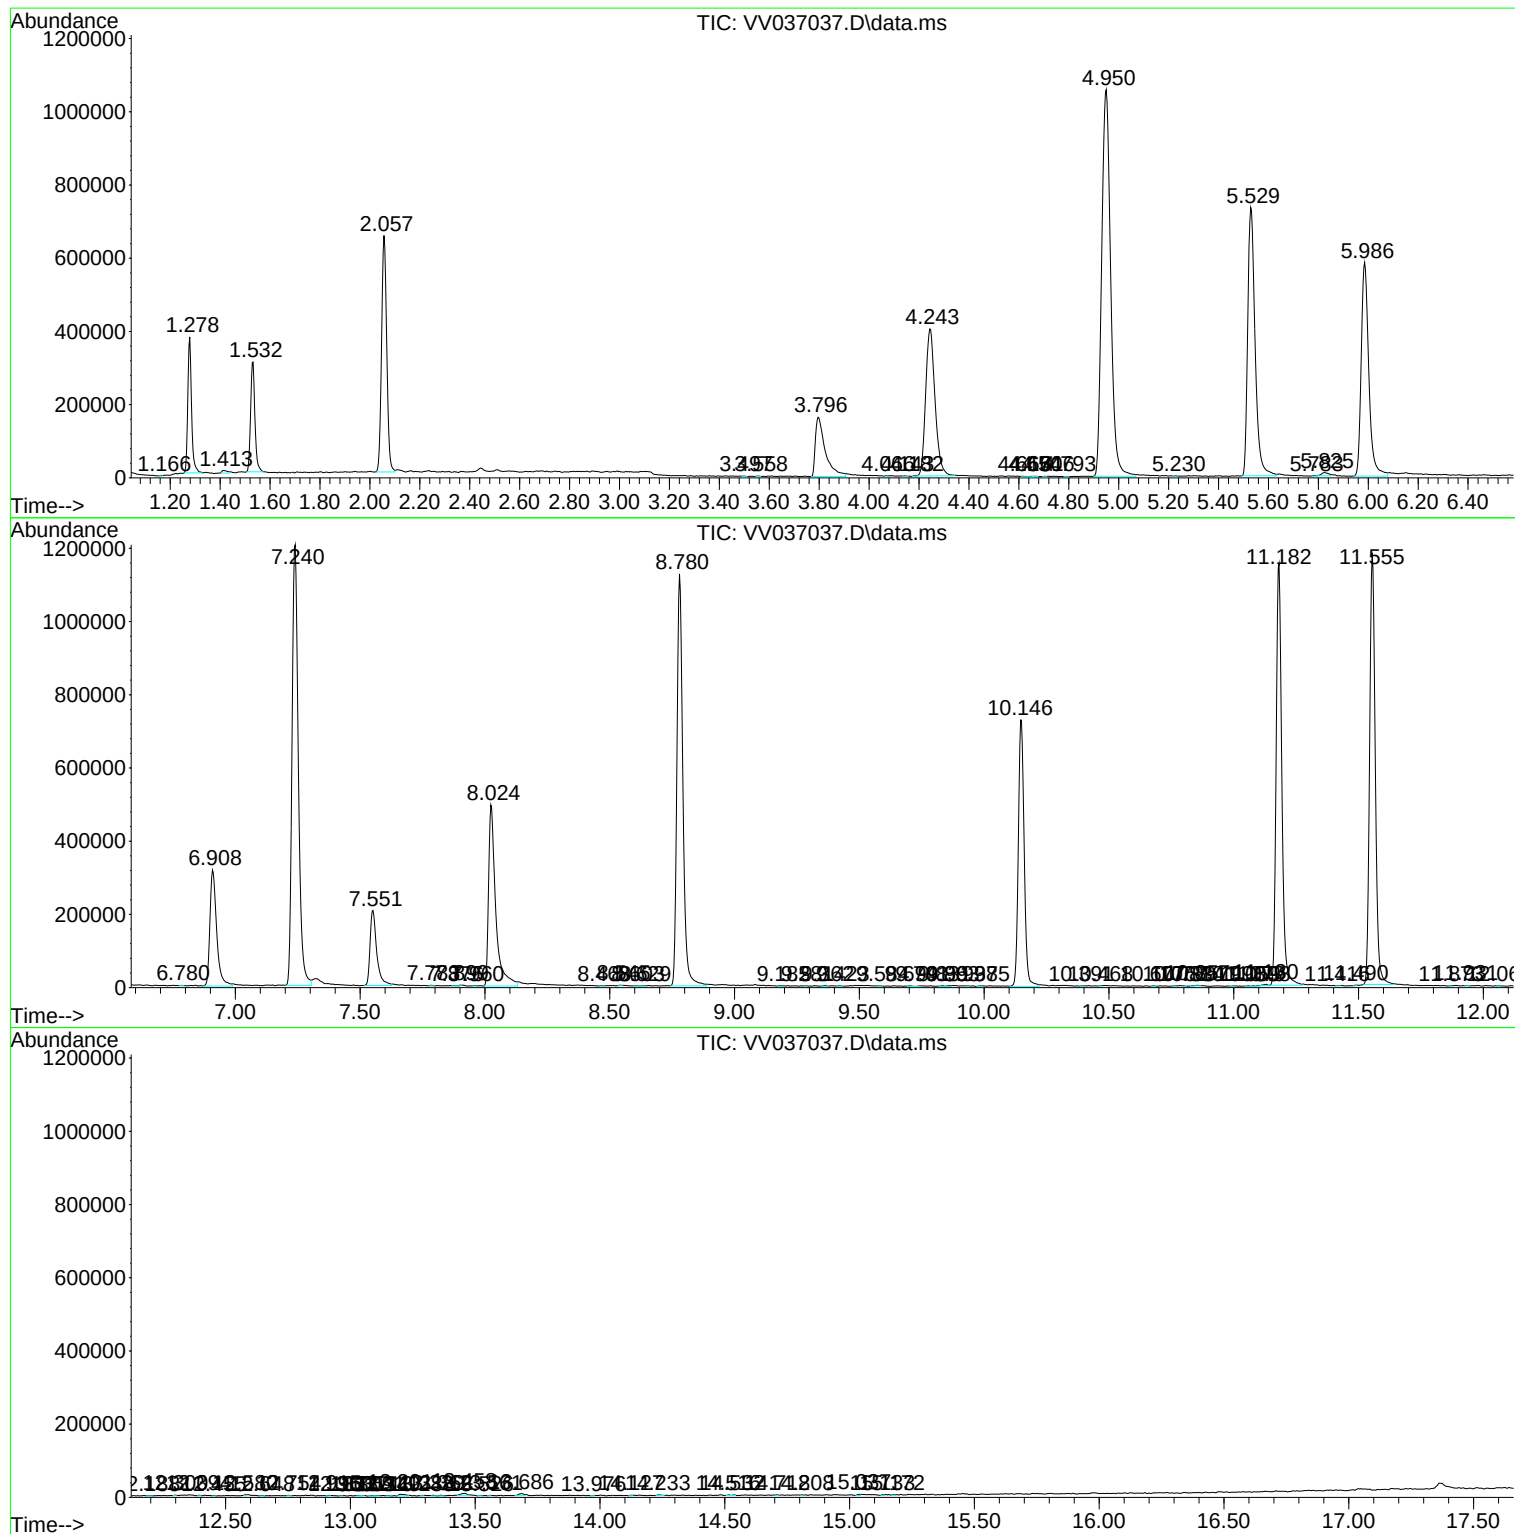

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037037.D
Acq On : 26 Aug 2024 18:51
Operator : SY/MD
Sample : P3692-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037037.D
Acq On : 26 Aug 2024 18:51
Operator : SY/MD
Sample : P3692-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc