

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037048.D
 Acq On : 26 Aug 2024 23:36
 Operator : SY/MD
 Sample : P3691-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	350005	367434	14.34%	2.015%
2	1.532	146	153	167	rVB	284383	341265	13.32%	1.871%
3	2.056	308	316	333	rVB	610574	862169	33.65%	4.728%
4	3.526	770	773	779	rBV6	1221	1277	0.05%	0.007%
5	3.629	802	805	806	rBV2	610	335	0.01%	0.002%
6	3.703	825	828	831	rVB4	1394	901	0.04%	0.005%
7	3.725	833	835	838	rVV4	692	360	0.01%	0.002%
8	3.796	848	857	886	rBV	142304	396712	15.48%	2.175%
9	4.243	981	996	1024	rBV2	387789	1004291	39.19%	5.507%
10	4.545	1084	1090	1094	rBV7	1808	1753	0.07%	0.010%
11	4.690	1132	1135	1137	rBV4	1622	1137	0.04%	0.006%
12	4.722	1143	1145	1146	rBV2	744	301	0.01%	0.002%
13	4.764	1155	1158	1160	rBV4	1613	914	0.04%	0.005%
14	4.831	1176	1179	1185	rVB7	1928	1897	0.07%	0.010%
15	4.857	1185	1187	1191	rVB5	868	501	0.02%	0.003%
16	4.876	1191	1193	1196	rBV4	1234	939	0.04%	0.005%
17	4.950	1200	1216	1253	rBV2	1013301	2562359	100.00%	14.051%
18	5.529	1385	1396	1429	rBV	672646	1397774	54.55%	7.665%
19	5.986	1525	1538	1567	rBV	571740	1169191	45.63%	6.411%
20	6.818	1795	1797	1803	rBV7	1498	1245	0.05%	0.007%
21	6.908	1815	1825	1855	rBV	280694	533414	20.82%	2.925%
22	7.240	1916	1928	1955	rBV	1146465	2028367	79.16%	11.123%
23	7.551	2016	2025	2047	rBV	180719	328675	12.83%	1.802%
24	8.027	2164	2173	2209	rBV	409031	849559	33.16%	4.659%
25	8.619	2354	2357	2359	rBV3	1551	1038	0.04%	0.006%
26	8.664	2369	2371	2372	rBV2	964	472	0.02%	0.003%
27	8.780	2396	2407	2443	rBV	1046189	1737691	67.82%	9.529%
28	9.175	2528	2530	2531	rBV2	1232	468	0.02%	0.003%
29	9.275	2557	2561	2570	rVB10	1916	2317	0.09%	0.013%
30	9.484	2620	2626	2631	rBV10	2073	2505	0.10%	0.014%
31	9.529	2636	2640	2641	rBV4	1352	1047	0.04%	0.006%
32	9.632	2671	2672	2675	rVB4	1900	766	0.03%	0.004%
33	9.686	2686	2689	2690	rBV3	613	339	0.01%	0.002%
34	9.699	2691	2693	2702	rVB8	1314	1396	0.05%	0.008%
35	9.934	2764	2766	2769	rVB3	1691	764	0.03%	0.004%
36	9.953	2769	2772	2775	rBV4	2523	1735	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037048.D
 Acq On : 26 Aug 2024 23:36
 Operator : SY/MD
 Sample : P3691-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.973	2775	2778	2779	rVV2	1271	796	0.03%	0.004%
38	9.995	2783	2785	2789	rVB5	1162	736	0.03%	0.004%
39	10.046	2798	2801	2803	rBV4	755	425	0.02%	0.002%
40	10.149	2821	2833	2857	rBV	692549	1095592	42.76%	6.008%
41	10.394	2907	2909	2911	rBV3	941	519	0.02%	0.003%
42	10.445	2921	2925	2928	rBV5	1417	1063	0.04%	0.006%
43	10.481	2933	2936	2938	rBV3	1612	1233	0.05%	0.007%
44	10.509	2943	2945	2947	rVV2	1017	358	0.01%	0.002%
45	10.625	2978	2981	2987	rVB7	1555	1343	0.05%	0.007%
46	10.657	2988	2991	2995	rVB6	1322	808	0.03%	0.004%
47	10.677	2995	2997	3001	rBV4	876	503	0.02%	0.003%
48	10.728	3010	3013	3017	rBV5	1212	901	0.04%	0.005%
49	10.757	3019	3022	3024	rVV4	1321	735	0.03%	0.004%
50	10.837	3045	3047	3049	rBV4	1043	542	0.02%	0.003%
51	10.850	3049	3051	3053	rVV3	1201	726	0.03%	0.004%
52	10.927	3073	3075	3076	rBV2	919	303	0.01%	0.002%
53	10.956	3080	3084	3085	rBV4	782	431	0.02%	0.002%
54	11.059	3111	3116	3121	rBV8	1663	1487	0.06%	0.008%
55	11.082	3121	3123	3125	rBV2	859	482	0.02%	0.003%
56	11.181	3143	3154	3180	rBV	1055564	1674609	65.35%	9.183%
57	11.506	3253	3255	3257	rBV3	821	377	0.01%	0.002%
58	11.554	3258	3270	3304	rVV	1117066	1819061	70.99%	9.975%
59	11.966	3396	3398	3400	rBV2	847	416	0.02%	0.002%
60	12.037	3418	3420	3421	rBV2	829	323	0.01%	0.002%
61	12.072	3429	3431	3433	rBV3	900	321	0.01%	0.002%
62	12.120	3444	3446	3448	rBV2	922	425	0.02%	0.002%
63	12.133	3448	3450	3452	rBV2	782	475	0.02%	0.003%
64	12.323	3507	3509	3510	rBV	526	223	0.01%	0.001%
65	12.397	3530	3532	3534	rBV3	1602	632	0.02%	0.003%
66	12.574	3582	3587	3588	rBV5	1169	1072	0.04%	0.006%
67	12.667	3609	3616	3618	rBV6	1904	1636	0.06%	0.009%
68	12.699	3624	3626	3627	rBV2	506	176	0.01%	0.001%
69	12.725	3630	3634	3635	rBV3	923	499	0.02%	0.003%
70	12.825	3663	3665	3670	rBV6	1500	1284	0.05%	0.007%
71	12.905	3686	3690	3694	rVB5	729	562	0.02%	0.003%
72	12.979	3711	3713	3715	rVB3	738	308	0.01%	0.002%
73	13.008	3720	3722	3724	rBV3	821	510	0.02%	0.003%
74	13.165	3768	3771	3774	rBV4	982	639	0.02%	0.004%
75	13.201	3775	3782	3785	rBV8	3217	4122	0.16%	0.023%
76	13.345	3825	3827	3828	rBV	1198	420	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037048.D
Acq On : 26 Aug 2024 23:36
Operator : SY/MD
Sample : P3691-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	13.361	3830	3832	3833	rBV2	1217	518	0.02%	0.003%
78	13.413	3846	3848	3852	rBV3	824	564	0.02%	0.003%
79	13.445	3852	3858	3861	rBV7	4129	4675	0.18%	0.026%
80	13.583	3899	3901	3904	rBV4	1383	685	0.03%	0.004%
81	13.660	3922	3925	3926	rBV3	1928	1011	0.04%	0.006%
82	13.760	3955	3956	3958	rVB2	1092	293	0.01%	0.002%
83	13.776	3958	3961	3963	rBV5	1160	589	0.02%	0.003%
84	13.828	3972	3977	3982	rVB7	2006	2149	0.08%	0.012%
85	13.850	3982	3984	3986	rBV3	904	603	0.02%	0.003%
86	13.972	4020	4022	4024	rBV3	1520	1028	0.04%	0.006%
87	14.085	4055	4057	4060	rBV3	1417	677	0.03%	0.004%
88	14.156	4076	4079	4082	rBV3	1584	1229	0.05%	0.007%
89	14.201	4090	4093	4097	rBV5	1834	1356	0.05%	0.007%
90	15.017	4345	4347	4349	rBV2	1282	592	0.02%	0.003%




Sum of corrected areas: 18236350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037048.D
Acq On : 26 Aug 2024 23:36
Operator : SY/MD
Sample : P3691-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

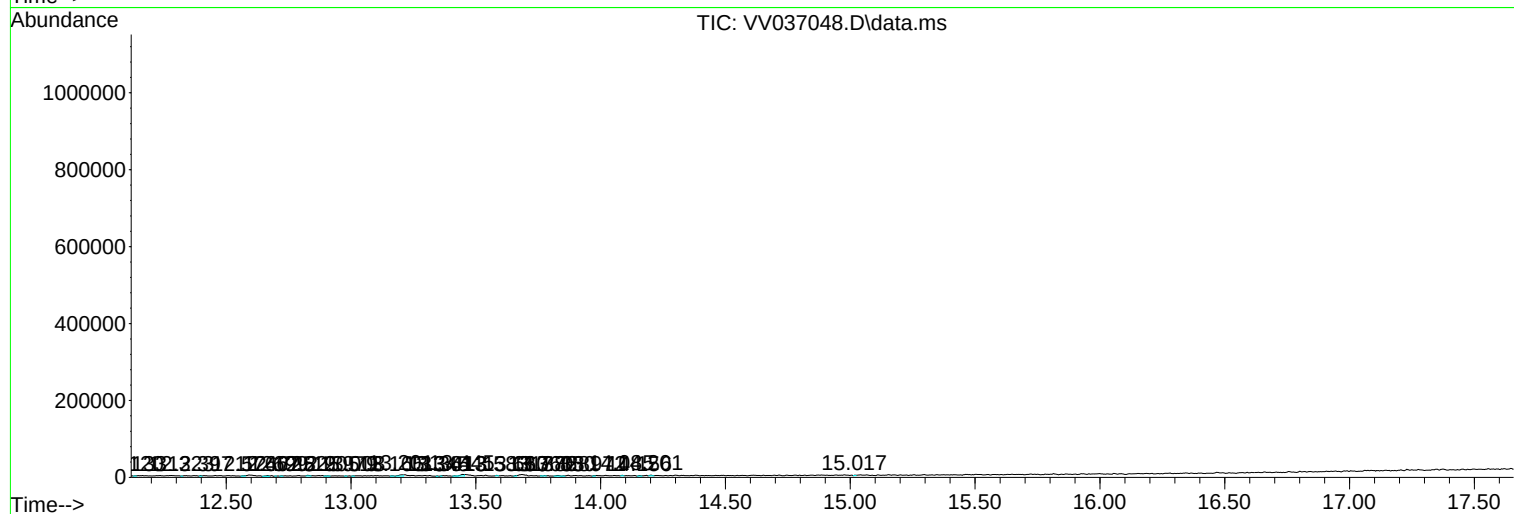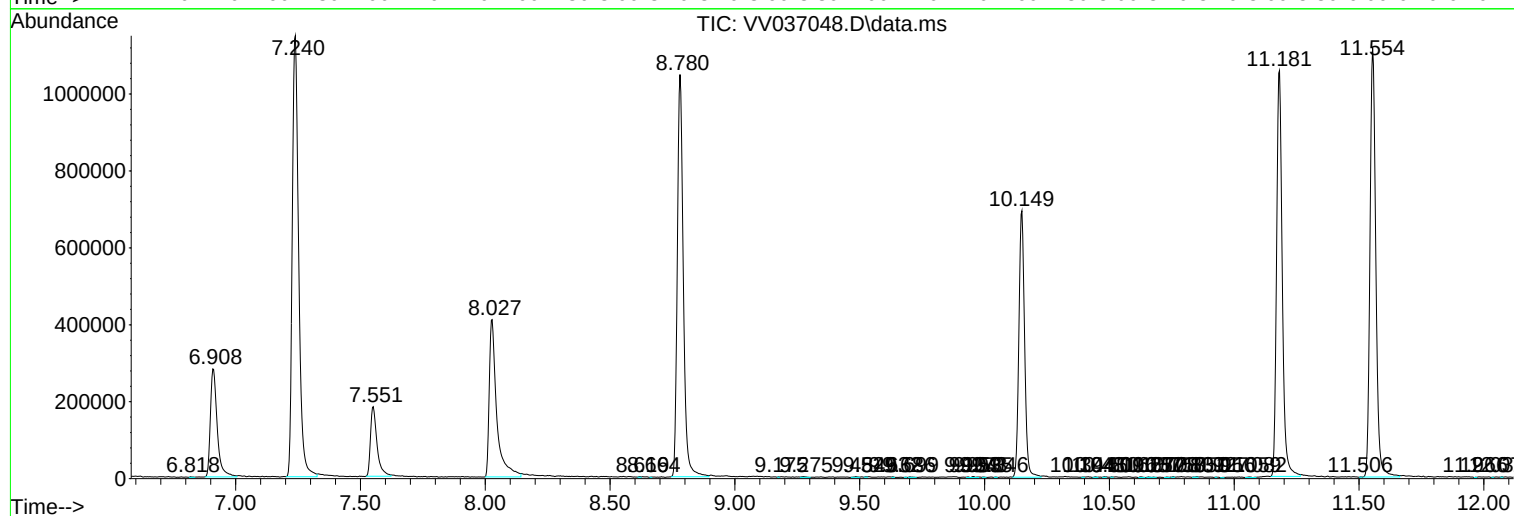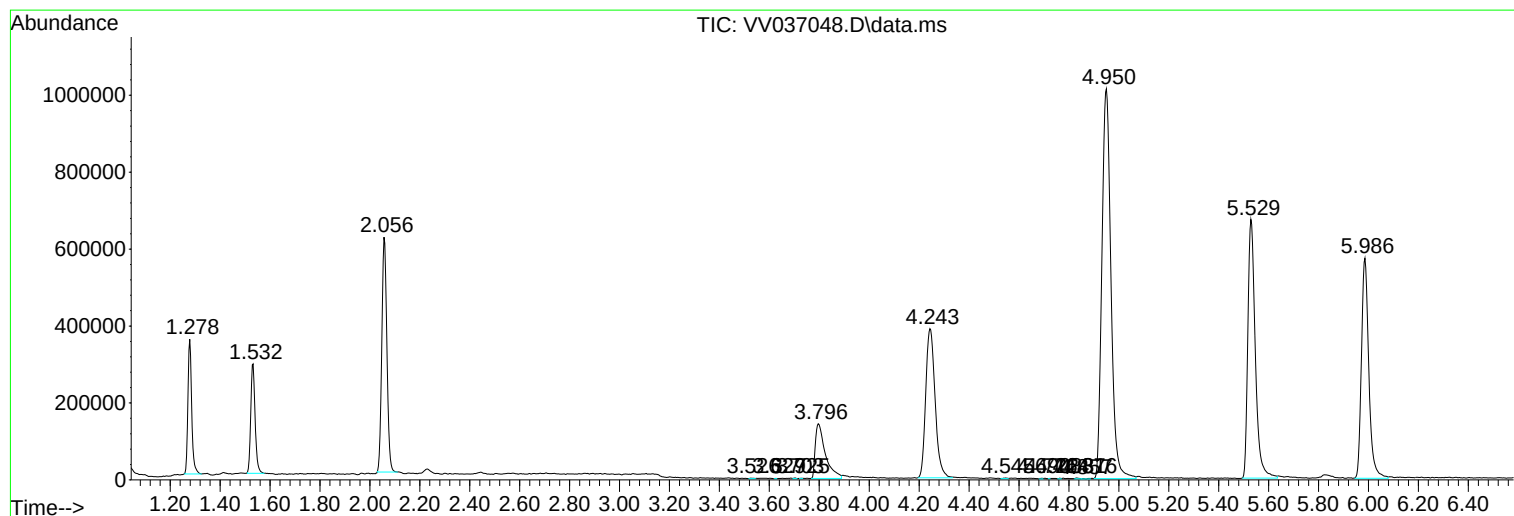

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037048.D
Acq On : 26 Aug 2024 23:36
Operator : SY/MD
Sample : P3691-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037048.D
Acq On : 26 Aug 2024 23:36
Operator : SY/MD
Sample : P3691-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------