

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037049.D
 Acq On : 26 Aug 2024 23:58
 Operator : SY/MD
 Sample : P3691-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	92	rVB	382007	404439	15.97%	2.279%
2	1.529	147	152	168	rVB	291139	351931	13.90%	1.983%
3	2.056	308	316	331	rVB	605476	864519	34.14%	4.872%
4	3.629	803	805	808	rBV3	1120	832	0.03%	0.005%
5	3.796	847	857	897	rBV	140238	398194	15.72%	2.244%
6	4.169	970	973	974	rBV3	904	577	0.02%	0.003%
7	4.243	982	996	1023	rBV	386945	990873	39.13%	5.584%
8	4.545	1086	1090	1092	rBV4	744	515	0.02%	0.003%
9	4.561	1092	1095	1099	rBV6	1812	1487	0.06%	0.008%
10	4.690	1131	1135	1136	rBV3	963	743	0.03%	0.004%
11	4.773	1158	1161	1162	rBV3	934	489	0.02%	0.003%
12	4.796	1166	1168	1171	rVB3	651	278	0.01%	0.002%
13	4.815	1171	1174	1175	rBV3	1027	440	0.02%	0.002%
14	4.825	1175	1177	1179	rBV3	428	203	0.01%	0.001%
15	4.883	1191	1195	1199	rBV7	1141	1029	0.04%	0.006%
16	4.950	1200	1216	1257	rBV2	1006023	2532279	100.00%	14.272%
17	5.310	1323	1328	1335	rBV8	1956	2330	0.09%	0.013%
18	5.529	1384	1396	1426	rBV	623200	1294603	51.12%	7.296%
19	5.931	1516	1521	1525	rBV8	1671	2061	0.08%	0.012%
20	5.985	1525	1538	1569	rVV	559162	1157740	45.72%	6.525%
21	6.908	1815	1825	1857	rBV	274853	529576	20.91%	2.985%
22	7.239	1916	1928	1951	rBV	1125492	1998111	78.91%	11.261%
23	7.551	2016	2025	2044	rBV	176194	322713	12.74%	1.819%
24	7.950	2146	2149	2151	rBV3	1430	755	0.03%	0.004%
25	8.024	2164	2172	2206	rBV	394451	820603	32.41%	4.625%
26	8.644	2362	2365	2367	rBV3	1701	997	0.04%	0.006%
27	8.780	2397	2407	2435	rBV	972250	1594080	62.95%	8.984%
28	9.275	2558	2561	2562	rBV3	826	561	0.02%	0.003%
29	9.329	2574	2578	2586	rBV10	1691	2342	0.09%	0.013%
30	9.535	2636	2642	2646	rBV8	2084	2451	0.10%	0.014%
31	9.680	2685	2687	2692	rVB5	1224	722	0.03%	0.004%
32	9.706	2692	2695	2697	rBV2	742	391	0.02%	0.002%
33	9.734	2702	2704	2705	rBV2	514	200	0.01%	0.001%
34	9.837	2733	2736	2739	rBV5	1114	769	0.03%	0.004%
35	9.857	2739	2742	2744	rBV4	1120	827	0.03%	0.005%
36	9.892	2750	2753	2757	rVB5	1488	1230	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037049.D
 Acq On : 26 Aug 2024 23:58
 Operator : SY/MD
 Sample : P3691-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.908	2757	2758	2760	rBV2	789	373	0.01%	0.002%
38	9.947	2767	2770	2776	rVB6	1778	1407	0.06%	0.008%
39	9.979	2776	2780	2783	rBV5	1510	1205	0.05%	0.007%
40	9.995	2783	2785	2787	rBV2	707	482	0.02%	0.003%
41	10.050	2801	2802	2804	rVB2	815	184	0.01%	0.001%
42	10.088	2811	2814	2815	rBV3	966	610	0.02%	0.003%
43	10.149	2820	2833	2849	rBV	671932	1072886	42.37%	6.047%
44	10.403	2909	2912	2923	rVB9	2208	3360	0.13%	0.019%
45	10.455	2923	2928	2929	rBV3	1782	1389	0.05%	0.008%
46	10.525	2946	2950	2954	rBV4	1539	1461	0.06%	0.008%
47	10.567	2961	2963	2965	rBV2	626	353	0.01%	0.002%
48	10.635	2982	2984	2985	rBV2	603	284	0.01%	0.002%
49	10.651	2985	2989	2995	rVB6	1510	1312	0.05%	0.007%
50	10.680	2995	2998	3002	rVB4	1449	1054	0.04%	0.006%
51	10.712	3002	3008	3011	rBV8	1463	1457	0.06%	0.008%
52	10.750	3017	3020	3021	rBV3	770	374	0.01%	0.002%
53	10.779	3025	3029	3033	rBV6	1644	1600	0.06%	0.009%
54	10.837	3043	3047	3051	rBV6	1281	1271	0.05%	0.007%
55	10.863	3051	3055	3056	rBV4	1077	857	0.03%	0.005%
56	10.911	3067	3070	3075	rBV5	1414	1337	0.05%	0.008%
57	10.998	3090	3097	3099	rBV7	1883	1923	0.08%	0.011%
58	11.040	3107	3110	3111	rBV	760	390	0.02%	0.002%
59	11.072	3116	3120	3122	rBV5	914	681	0.03%	0.004%
60	11.117	3129	3134	3135	rBV4	1702	1510	0.06%	0.009%
61	11.181	3143	3154	3183	rBV	970873	1546936	61.09%	8.718%
62	11.554	3257	3270	3301	rBV	1100298	1794697	70.87%	10.115%
63	11.940	3389	3390	3394	rBV5	652	485	0.02%	0.003%
64	12.117	3438	3445	3450	rVB10	1172	1648	0.07%	0.009%
65	12.152	3454	3456	3458	rBV3	809	409	0.02%	0.002%
66	12.185	3464	3466	3469	rVB4	1593	585	0.02%	0.003%
67	12.242	3482	3484	3485	rBV2	942	398	0.02%	0.002%
68	12.294	3497	3500	3503	rBV5	1246	770	0.03%	0.004%
69	12.471	3550	3555	3559	rBV7	2167	1712	0.07%	0.010%
70	12.529	3571	3573	3575	rVB3	947	316	0.01%	0.002%
71	12.541	3575	3577	3582	rVB5	798	676	0.03%	0.004%
72	12.622	3600	3602	3604	rBV3	916	293	0.01%	0.002%
73	12.667	3612	3616	3619	rBV4	1408	1157	0.05%	0.007%
74	12.754	3640	3643	3649	rBV7	1686	2005	0.08%	0.011%
75	12.792	3653	3655	3656	rBV	819	220	0.01%	0.001%
76	13.091	3746	3748	3751	rBV4	872	556	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
 Data File : VV037049.D
 Acq On : 26 Aug 2024 23:58
 Operator : SY/MD
 Sample : P3691-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1K46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	13.127	3756	3759	3762	rVB3	1039	550	0.02%	0.003%
78	13.146	3762	3765	3768	rBV5	1725	938	0.04%	0.005%
79	13.168	3768	3772	3777	rBV6	975	817	0.03%	0.005%
80	13.201	3777	3782	3783	rBV5	2861	2450	0.10%	0.014%
81	13.811	3968	3972	3975	rBV5	1028	1017	0.04%	0.006%
82	13.860	3985	3987	3989	rBV2	1138	663	0.03%	0.004%
83	14.069	4050	4052	4053	rBV	1109	534	0.02%	0.003%
84	14.326	4129	4132	4133	rBV2	990	617	0.02%	0.003%
85	14.403	4154	4156	4158	rBV2	1111	501	0.02%	0.003%
86	14.635	4226	4228	4234	rVB4	1935	1847	0.07%	0.010%
87	14.667	4234	4238	4239	rBV3	1766	1029	0.04%	0.006%




Sum of corrected areas: 17743476

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037049.D
Acq On : 26 Aug 2024 23:58
Operator : SY/MD
Sample : P3691-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

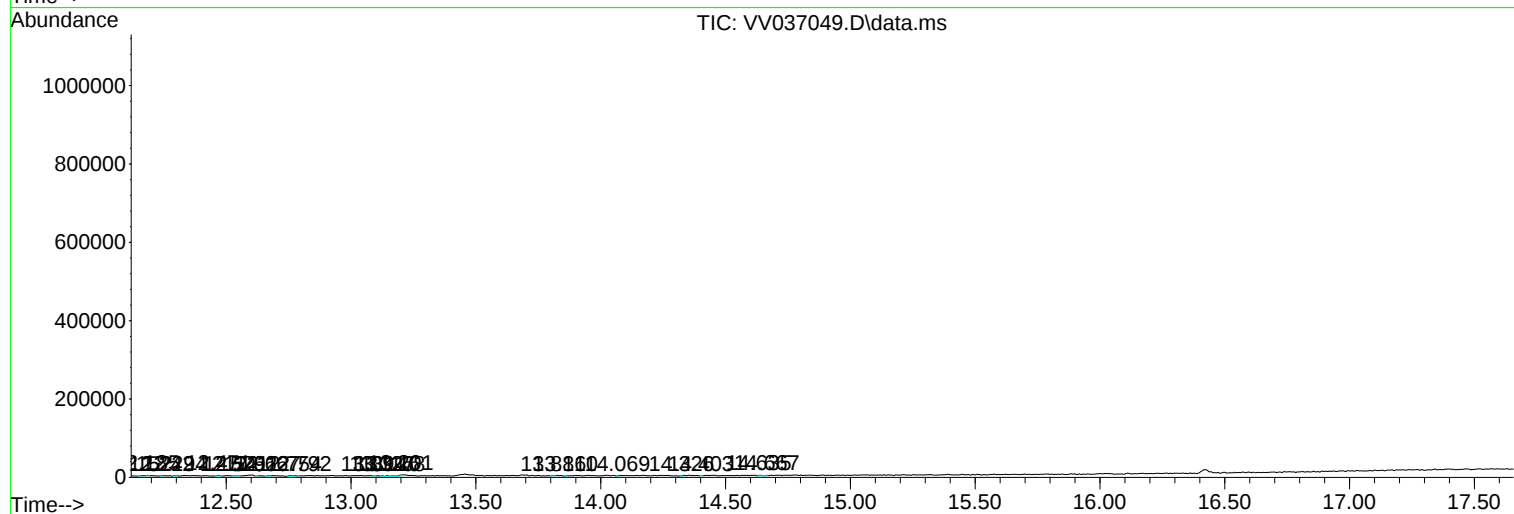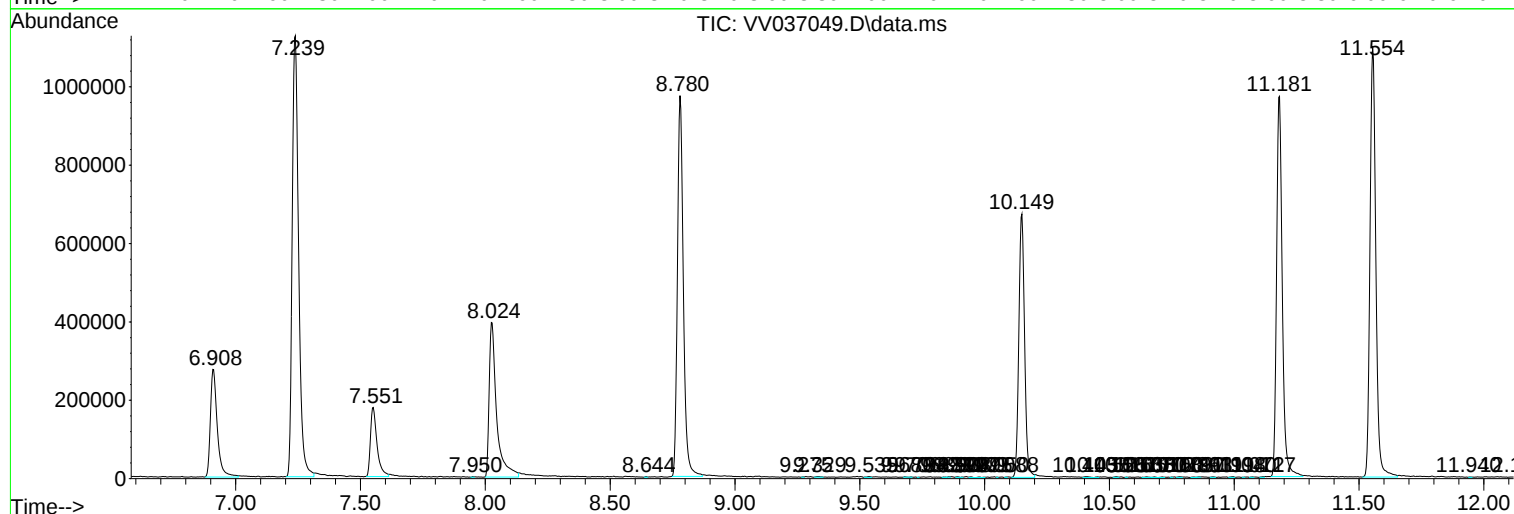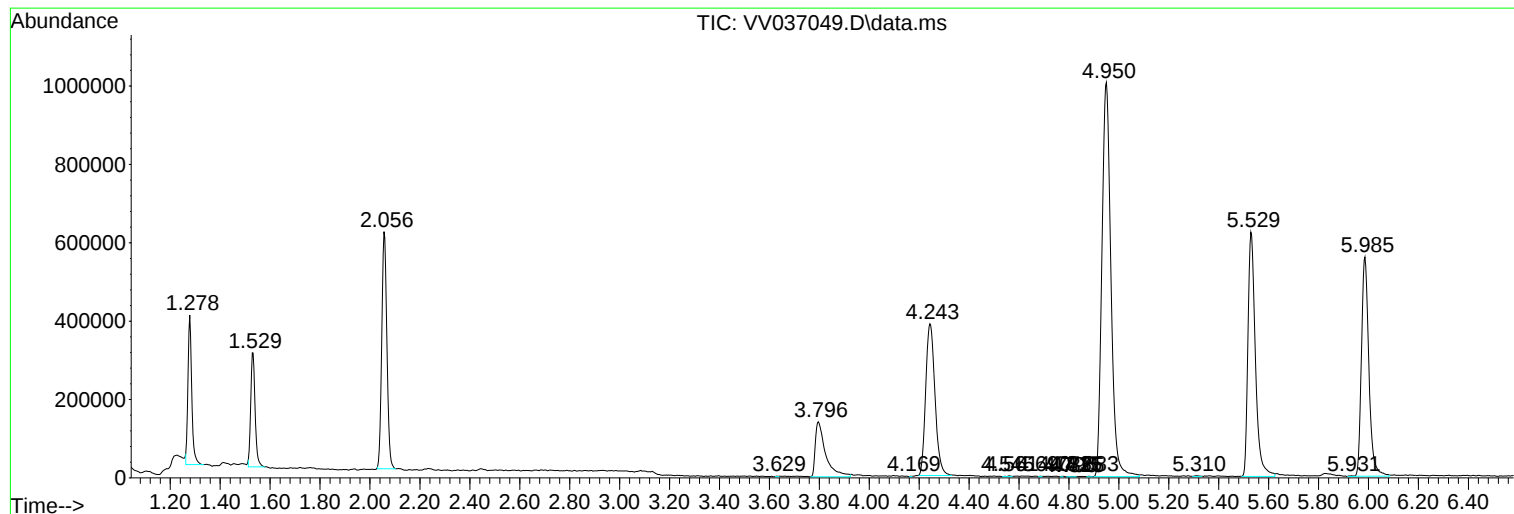

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037049.D
Acq On : 26 Aug 2024 23:58
Operator : SY/MD
Sample : P3691-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037049.D
Acq On : 26 Aug 2024 23:58
Operator : SY/MD
Sample : P3691-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1K46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
