
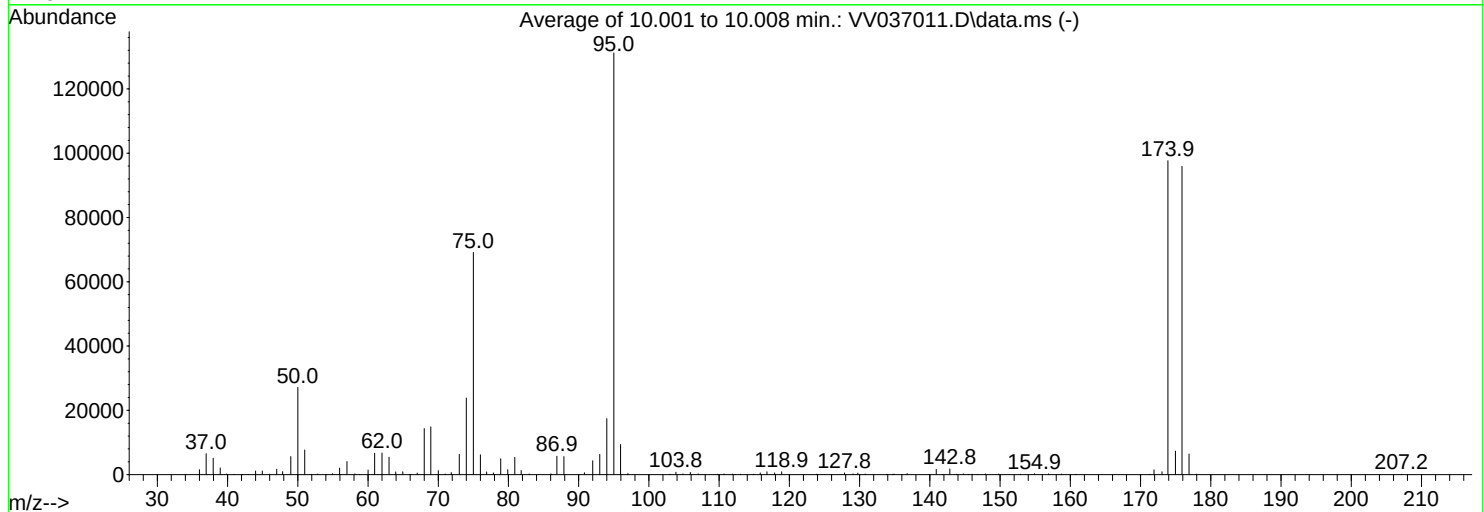


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082624\
Data File : VV037011.D
Acq On : 26 Aug 2024 08:36
Operator : SY/MD
Sample : BFB368
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB368

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Thu Aug 29 04:43:38 2024

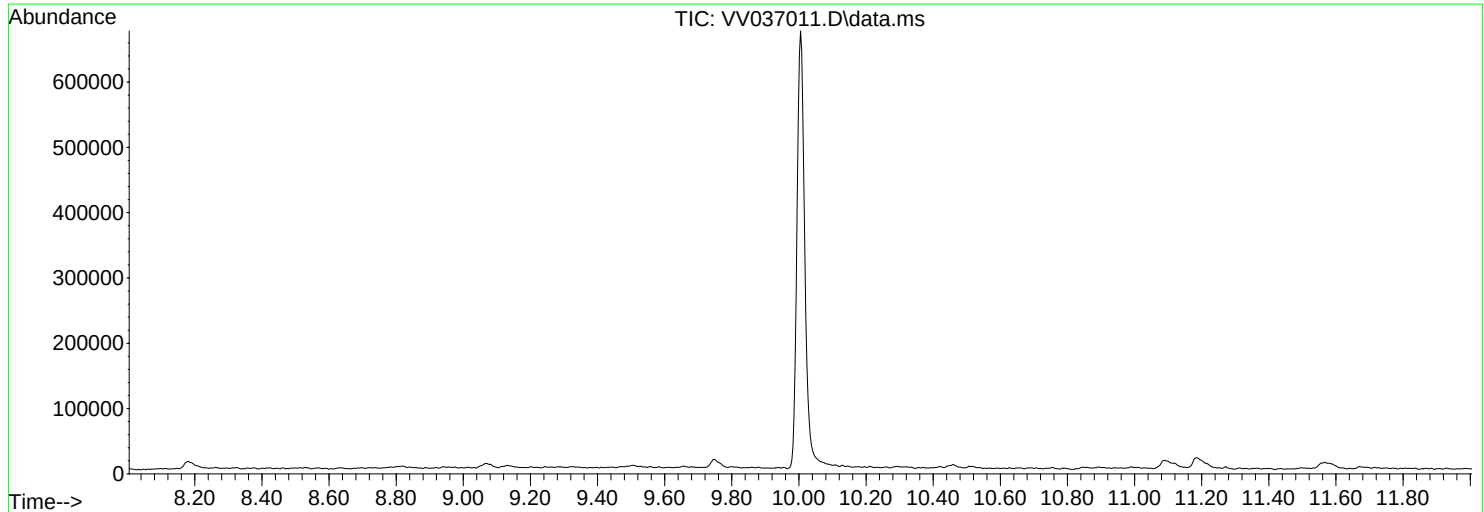

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	27112	PASS
75	95	30	80	52.7	69120	PASS
95	95	100	100	100.0	131219	PASS
96	95	5	9	7.1	9371	PASS
173	174	0.00	2	0.9	895	PASS
174	95	50	120	74.4	97669	PASS
175	174	5	9	7.5	7303	PASS
176	174	95	105	98.2	95923	PASS
177	176	5	10	6.7	6442	PASS

m/z	Abundance
36.00	2940.0
36.90	297.0
37.90	1255.0
38.90	327.0
39.90	345.0
41.00	275.0
42.10	179.0
43.00	306.0
44.00	691.0
44.80	133.0
51.90	172.0
54.10	130.0
55.10	271.0
55.90	117.0
57.00	148.0
59.10	116.0
68.90	133.0
76.90	162.0
95.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	4553.0
37.00	6665.0
38.00	6248.0
39.00	2450.0
39.90	534.0
40.90	374.0
42.10	150.0
43.00	368.0
44.00	1834.0
45.00	1358.0
46.00	164.0
47.00	1695.0
47.80	960.0
49.00	5402.0
50.00	26928.0
51.00	7671.0
51.90	281.0
52.80	212.0
53.80	186.0
54.90	510.0
56.00	2162.0
57.00	4477.0
58.20	272.0
60.00	1505.0
60.90	6678.0
62.00	6661.0
63.00	5333.0
64.00	791.0
65.00	972.0
65.90	171.0
67.00	403.0
68.00	14498.0
69.00	14450.0
70.00	1210.0
71.00	242.0
71.90	637.0
73.00	6132.0
74.00	23592.0
75.00	68832.0
76.00	5914.0
76.90	940.0
77.90	587.0
78.90	4890.0
79.90	1579.0
80.90	5276.0
81.80	1179.0
83.00	265.0
86.00	317.0
86.90	5624.0
87.90	5765.0
90.80	594.0
92.00	4239.0
93.00	6316.0
94.00	16357.0
95.00	127624.0
96.00	9661.0
97.00	344.0
103.00	190.0
103.80	766.0
104.80	259.0
105.90	691.0
107.00	250.0
109.80	146.0
110.70	240.0
111.90	151.0
112.30	112.0
113.00	178.0
114.90	153.0
115.90	523.0
116.80	1009.0
117.90	543.0
118.90	949.0
123.90	174.0
127.80	560.0
129.10	223.0
129.80	496.0
130.80	286.0
133.80	108.0
134.70	261.0
136.80	314.0
140.90	1492.0
141.80	105.0
142.80	1953.0
143.70	106.0
144.80	277.0
146.00	156.0
146.80	153.0
147.90	225.0
149.80	178.0
153.00	118.0
154.90	291.0
156.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

156.90	273.0
158.80	219.0
160.80	159.0
171.30	327.0
171.90	1364.0
173.00	1241.0
173.90	94096.0
174.90	7334.0
175.90	92120.0
176.90	6261.0
177.90	148.0
207.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	4608.0
37.00	7076.0
38.00	6496.0
39.00	2501.0
40.00	556.0
40.90	382.0
41.90	186.0
43.00	360.0
44.00	1846.0
45.00	1298.0
46.00	158.0
47.00	1738.0
47.80	962.0
49.00	5925.0
50.00	27920.0
51.00	7910.0
51.90	308.0
52.80	206.0
53.90	160.0
54.90	600.0
56.00	2266.0
57.00	4410.0
58.20	253.0
60.00	1539.0
61.00	6908.0
62.00	6821.0
63.00	5592.0
63.90	888.0
65.00	898.0
65.90	155.0
67.00	518.0
68.00	14874.0
69.00	15619.0
70.00	1329.0
71.00	208.0
71.80	655.0
73.00	6560.0
74.00	24456.0
75.00	71376.0
76.00	6396.0
76.90	1070.0
77.90	579.0
78.90	5218.0
79.90	1606.0
80.90	5581.0
81.80	1325.0
83.00	209.0
86.00	256.0
86.90	5905.0
87.90	5863.0
90.80	632.0
92.00	4507.0
93.00	6568.0
94.00	18080.0
95.00	135552.0
96.00	9798.0
97.00	379.0
103.00	194.0
103.90	743.0
104.90	277.0
105.90	712.0
107.00	260.0
109.80	160.0
110.70	257.0
111.90	184.0
113.10	142.0
114.90	156.0
115.80	606.0
116.80	907.0
117.90	585.0
118.90	944.0
123.80	173.0
124.90	107.0
127.90	534.0
129.00	244.0
129.80	528.0
130.80	212.0
133.80	124.0
134.90	310.0
136.80	347.0
140.90	1713.0
142.80	1829.0
143.70	147.0
144.70	266.0
145.50	128.0
146.00	185.0
146.80	123.0
147.90	227.0
149.80	211.0
152.90	171.0
154.90	292.0
156.90	261.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

158.70	231.0
160.80	159.0
171.90	1561.0
173.10	1443.0
173.90	100992.0
174.90	7538.0
175.90	98936.0
176.90	6639.0
178.00	171.0
207.20	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	4335.0
37.00	6666.0
38.00	6412.0
39.00	2357.0
40.00	572.0
41.00	384.0
41.90	238.0
42.90	304.0
44.00	1797.0
45.00	1197.0
46.00	137.0
47.00	1620.0
47.90	935.0
49.00	5511.0
50.00	26488.0
51.00	7505.0
51.90	303.0
52.80	201.0
54.00	122.0
55.00	633.0
56.00	2090.0
57.00	3772.0
58.10	223.0
58.80	108.0
60.00	1367.0
60.90	6363.0
62.00	6670.0
63.00	5327.0
63.90	833.0
64.90	860.0
66.10	145.0
67.00	576.0
68.00	13702.0
69.00	14968.0
70.00	1191.0
71.10	123.0
71.90	620.0
73.00	6270.0
74.00	23496.0
75.00	67152.0
76.00	6244.0
76.90	1047.0
77.80	496.0
78.90	4761.0
79.90	1505.0
80.90	5246.0
81.80	1324.0
82.90	184.0
86.10	229.0
86.90	5684.0
87.90	5327.0
90.80	574.0
92.00	4235.0
93.00	6093.0
94.00	17784.0
95.00	130480.0
96.00	8982.0
97.00	375.0
103.00	131.0
103.90	729.0
104.90	243.0
105.90	680.0
107.00	200.0
109.80	157.0
110.70	207.0
111.90	232.0
113.00	125.0
114.90	152.0
115.80	566.0
116.80	776.0
117.90	539.0
118.90	868.0
123.80	165.0
125.00	100.0
127.90	529.0
129.00	253.0
129.70	445.0
130.80	156.0
133.80	110.0
134.90	335.0
136.70	325.0
140.00	112.0
140.90	1669.0
142.90	1550.0
143.80	169.0
144.70	244.0
145.50	174.0
146.00	178.0
146.80	103.0
147.90	245.0
149.80	207.0
152.80	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

154.90	331.0
156.90	228.0
158.70	165.0
160.80	143.0
171.90	1584.0
173.90	97920.0
175.00	7038.0
175.90	96712.0
176.90	6426.0
177.90	206.0
207.20	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368