


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082718\
Data File : VV007211.D
Acq On : 27 Aug 2018 10:12
Operator : SY/MD
Sample : BFB66
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB66

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082118WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Aug 28 01:40:53 2018

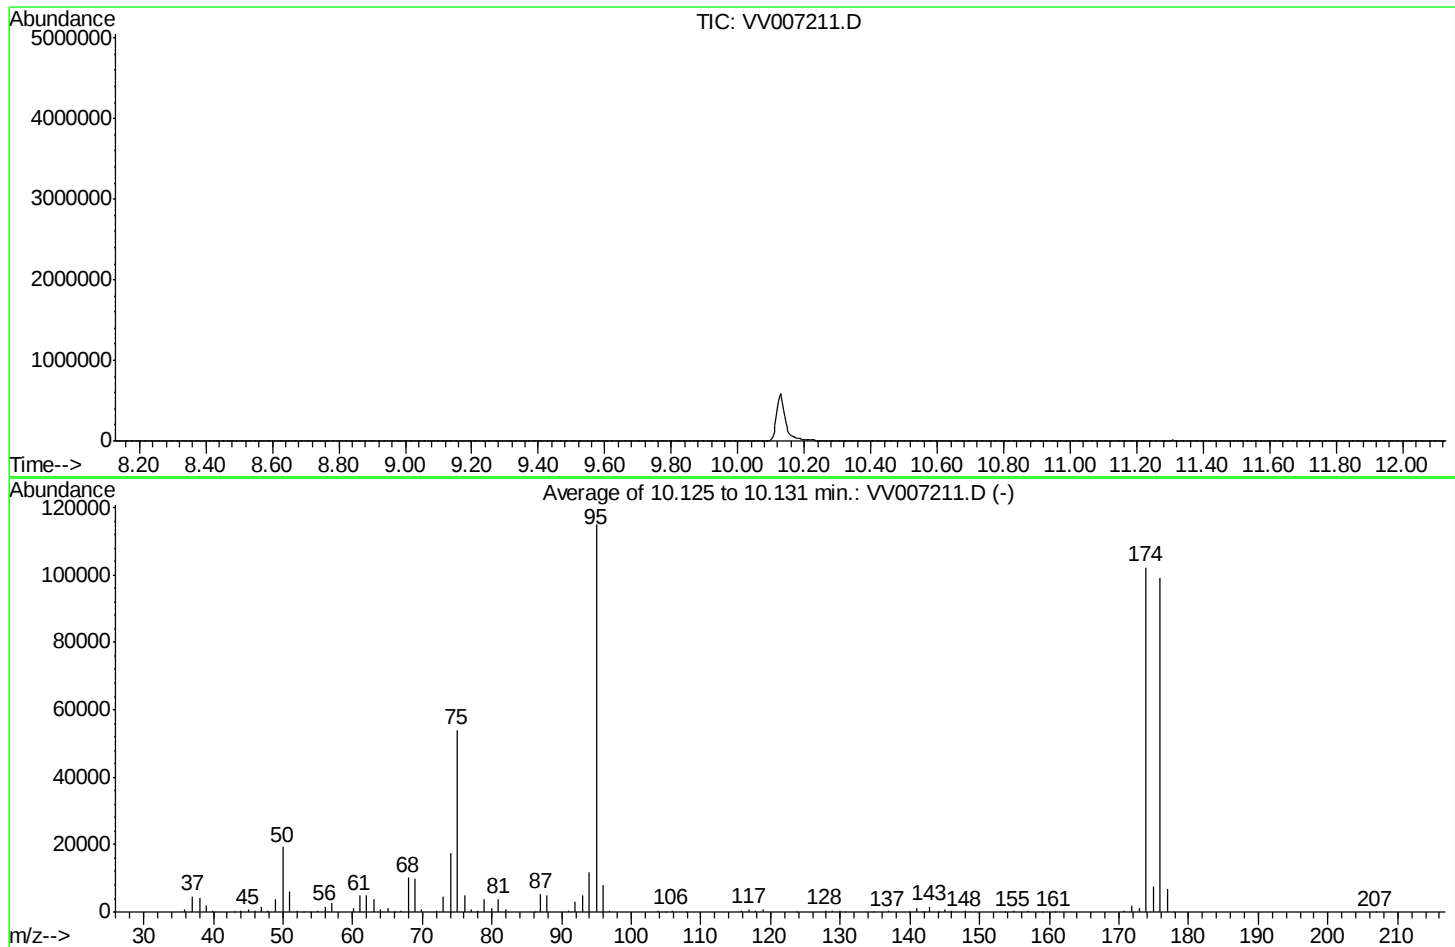

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	19362	PASS
75	95	30	80	47.0	54058	PASS
95	95	100	100	100.0	115045	PASS
96	95	5	9	6.8	7878	PASS
173	174	0.00	2	1.3	1295	PASS
174	95	50	120	88.9	102232	PASS
175	174	5	9	7.3	7478	PASS
176	174	95	101	96.9	99104	PASS
177	176	5	9	6.9	6859	PASS

Scan 2859 (10.083 min): VV007211.D
BFB66

m/z	Abundance
39.80	392.0
44.00	1021.0
45.10	116.0
206.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	887.0
37.00	4662.0
38.00	4252.0
39.10	1947.0
39.90	701.0
44.00	1470.0
45.00	851.0
45.90	207.0
47.00	1509.0
47.90	506.0
49.00	4107.0
50.00	19272.0
51.00	6161.0
52.00	249.0
52.90	174.0
54.00	166.0
54.90	288.0
56.00	1578.0
57.00	2725.0
60.10	1043.0
61.00	4951.0
62.00	4946.0
63.00	3593.0
64.00	712.0
65.00	1178.0
67.00	266.0
68.00	10041.0
69.00	10208.0
69.90	758.0
72.00	554.0
73.00	4579.0
74.00	17672.0
75.00	53672.0
76.10	5366.0
77.00	793.0
77.90	444.0
78.90	3906.0
79.90	1171.0
80.90	3861.0
81.90	834.0
86.20	131.0
87.00	5605.0
88.00	4783.0
91.00	452.0
92.00	2913.0
93.00	5077.0
94.00	12347.0
95.00	115968.0
96.00	8062.0
96.90	283.0
103.90	439.0
104.90	109.0
105.80	426.0
107.90	172.0
115.80	332.0
116.90	778.0
117.80	314.0
118.90	643.0
123.70	126.0
127.80	506.0
128.80	250.0
129.90	426.0
130.70	112.0
134.80	155.0
136.90	212.0
139.80	121.0
140.90	906.0
142.10	151.0
142.90	1635.0
144.00	122.0
144.90	746.0
145.90	323.0
147.90	299.0
153.70	148.0
154.80	276.0
157.00	212.0
159.00	143.0
160.80	147.0
170.80	377.0
171.90	1825.0
172.90	1227.0
173.90	99944.0
174.90	7363.0
175.90	96976.0
176.90	6546.0
177.90	132.0
207.00	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	918.0
37.00	4911.0
38.00	4428.0
39.10	2152.0
39.90	677.0
43.10	108.0
44.00	1413.0
45.00	865.0
45.90	215.0
46.90	1469.0
47.90	446.0
49.00	3980.0
50.00	20000.0
51.00	6429.0
52.00	255.0
52.90	182.0
53.90	167.0
54.90	339.0
56.00	1620.0
57.00	2722.0
60.00	1106.0
61.00	5068.0
62.00	4984.0
63.00	3832.0
64.00	704.0
65.00	1256.0
66.00	129.0
67.00	265.0
68.00	10429.0
69.00	10130.0
69.90	817.0
72.00	568.0
73.00	4723.0
74.00	18264.0
75.00	56088.0
76.10	5118.0
76.90	819.0
78.00	403.0
78.90	3772.0
79.90	1391.0
80.90	4090.0
81.90	864.0
87.00	5514.0
87.90	4858.0
91.00	489.0
91.90	2992.0
93.00	5292.0
94.00	12208.0
95.00	118544.0
96.00	8147.0
96.90	255.0
103.90	449.0
104.90	102.0
105.80	453.0
107.90	127.0
115.90	366.0
116.90	883.0
117.80	363.0
118.90	725.0
123.70	124.0
127.90	508.0
128.80	262.0
129.90	427.0
130.70	114.0
134.80	175.0
136.90	216.0
139.80	165.0
140.90	1030.0
141.80	189.0
142.90	1779.0
144.00	101.0
145.00	838.0
145.90	308.0
147.90	371.0
153.70	141.0
154.80	229.0
157.00	233.0
159.00	140.0
160.80	161.0
170.80	405.0
171.90	1804.0
172.90	1345.0
173.90	105320.0
174.90	7687.0
175.90	102008.0
176.90	7145.0
177.90	138.0
206.90	157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
35.90	919.0
37.00	4604.0
38.00	4078.0
39.00	2012.0
39.90	624.0
43.10	108.0
44.00	1403.0
45.00	786.0
45.90	234.0
47.00	1420.0
47.90	405.0
49.00	3573.0
50.00	18816.0
51.00	6136.0
51.90	279.0
52.90	133.0
54.00	125.0
54.90	367.0
56.00	1464.0
57.00	2507.0
60.00	1112.0
61.00	4700.0
62.00	4748.0
63.00	3795.0
64.00	721.0
65.00	1358.0
66.00	131.0
66.90	254.0
68.00	10215.0
69.00	9416.0
69.90	737.0
72.00	535.0
73.00	4450.0
74.00	17032.0
75.00	52416.0
76.10	4161.0
76.90	758.0
77.90	357.0
78.90	3564.0
79.90	1364.0
80.90	3902.0
81.90	848.0
86.90	5124.0
87.90	4705.0
91.00	444.0
92.00	2986.0
93.00	4837.0
94.00	10986.0
95.00	110624.0
96.00	7425.0
97.00	162.0
103.90	400.0
105.80	471.0
115.90	418.0
116.90	869.0
117.80	353.0
118.90	731.0
123.70	111.0
127.90	401.0
128.90	224.0
129.90	386.0
130.80	144.0
134.80	128.0
136.90	206.0
139.80	166.0
140.90	1034.0
141.80	210.0
142.80	1731.0
144.90	867.0
145.90	238.0
147.90	350.0
154.90	226.0
157.00	239.0
158.90	144.0
160.80	136.0
170.80	394.0
171.90	1624.0
172.90	1313.0
173.90	101432.0
174.90	7384.0
175.90	98328.0
176.90	6887.0
177.90	141.0
206.90	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66