


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082719\
Data File : VV012413.D
Acq On : 27 Aug 2019 08:15
Operator : SY/MD
Sample : BFB54
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB54

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Sep 09 09:09:55 2019

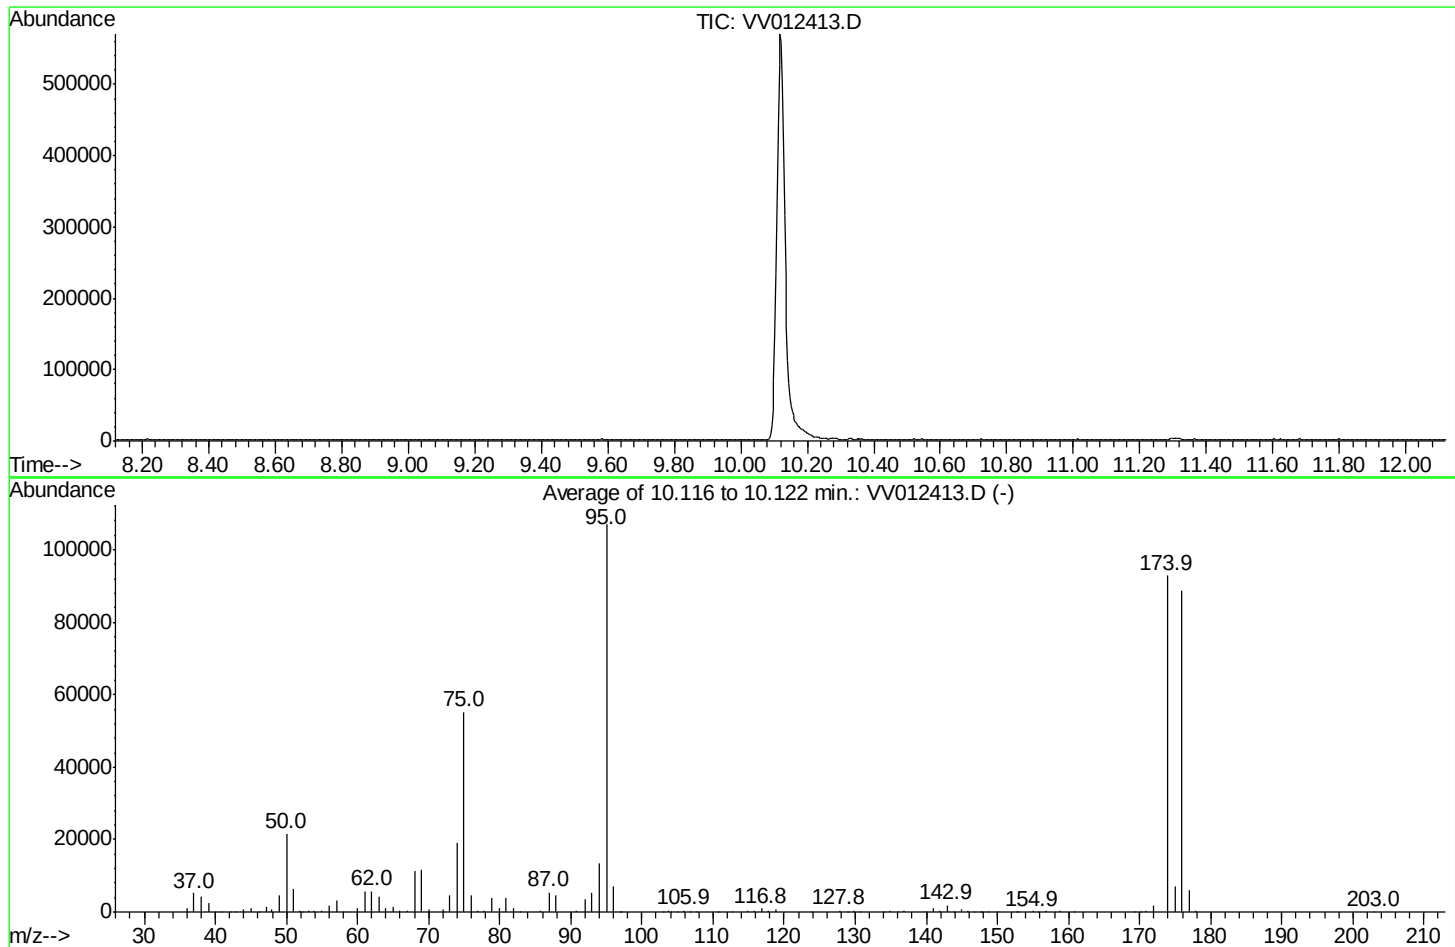

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	21743	PASS
75	95	30	80	51.5	55138	PASS
95	95	100	100	100.0	107032	PASS
96	95	5	9	6.5	6959	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.7	92840	PASS
175	174	5	9	7.5	6955	PASS
176	174	95	101	95.6	88738	PASS
177	176	5	9	6.7	5922	PASS

Scan 2794 (10.074 min): VV012413.D
BFB54

m/z	Abundance
35.80	119.0
37.00	108.0
37.90	120.0
39.90	829.0
44.00	528.0
46.30	103.0
50.10	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	972.0
37.00	5257.0
38.00	4601.0
39.00	2386.0
40.00	979.0
40.90	124.0
43.90	1262.0
44.90	1021.0
46.10	181.0
47.10	1637.0
47.90	601.0
49.00	4354.0
50.00	21392.0
51.00	6226.0
52.20	330.0
53.10	188.0
53.90	210.0
54.80	344.0
56.00	1730.0
57.00	2896.0
58.00	174.0
60.00	964.0
61.00	5519.0
62.00	5463.0
63.00	4120.0
64.00	861.0
65.00	1477.0
65.90	228.0
66.90	425.0
68.00	10670.0
69.00	11490.0
70.00	817.0
72.10	649.0
73.00	4611.0
74.00	18640.0
75.00	53192.0
76.00	4241.0
76.90	440.0
77.90	504.0
78.90	3670.0
80.00	1078.0
80.90	3807.0
82.00	946.0
82.90	162.0
85.80	272.0
87.00	5259.0
87.90	4332.0
90.80	434.0
92.00	3228.0
93.00	5098.0
94.00	12749.0
95.00	103088.0
96.00	6608.0
96.90	155.0
103.00	112.0
103.80	363.0
105.00	142.0
105.90	521.0
106.80	126.0
110.70	121.0
112.80	131.0
114.80	185.0
115.90	421.0
116.90	844.0
117.70	322.0
118.80	760.0
127.80	449.0
128.90	138.0
129.90	431.0
130.70	151.0
134.80	237.0
136.80	186.0
140.00	134.0
140.90	950.0
142.00	148.0
142.90	1842.0
143.90	179.0
144.90	521.0
145.80	174.0
147.60	184.0
148.80	115.0
152.60	150.0
154.90	254.0
156.90	181.0
158.80	192.0
160.70	154.0
170.90	329.0
171.90	1614.0
173.90	87240.0
175.00	6676.0
175.90	82688.0
176.90	5589.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

177.90

220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	1176.0
37.00	5559.0
38.00	4630.0
39.00	2518.0
39.90	949.0
40.90	143.0
42.90	129.0
43.90	1305.0
44.90	1112.0
46.10	237.0
47.10	1549.0
47.90	635.0
49.00	4778.0
50.00	22616.0
51.00	6583.0
51.90	346.0
53.10	194.0
53.90	242.0
54.90	369.0
56.00	1765.0
57.00	3180.0
57.90	143.0
60.00	1053.0
61.00	5846.0
62.00	5839.0
63.00	4577.0
64.00	945.0
65.00	1631.0
65.90	235.0
66.90	422.0
68.00	11582.0
69.00	12127.0
70.00	806.0
72.00	657.0
73.00	4937.0
74.00	19784.0
75.00	57032.0
76.00	4671.0
77.00	519.0
77.80	518.0
78.90	3938.0
80.00	1152.0
80.90	4032.0
82.00	1002.0
82.90	112.0
85.80	285.0
87.00	5642.0
87.90	4883.0
90.70	416.0
92.00	3516.0
93.00	5292.0
94.00	13886.0
95.00	110280.0
96.00	7105.0
97.10	198.0
103.00	101.0
103.80	371.0
104.90	161.0
105.90	498.0
106.80	162.0
110.80	114.0
114.80	196.0
115.80	401.0
116.90	986.0
117.80	357.0
118.80	844.0
127.80	519.0
128.80	184.0
129.90	481.0
130.80	160.0
133.90	127.0
134.90	254.0
136.00	106.0
136.90	216.0
139.90	147.0
140.90	1072.0
141.90	215.0
142.90	1956.0
143.90	192.0
144.90	587.0
145.80	207.0
146.80	111.0
147.70	177.0
148.80	146.0
150.00	123.0
152.80	132.0
155.00	301.0
155.70	117.0
156.90	273.0
158.70	202.0
160.70	192.0
170.20	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

170.90	418.0
171.90	1804.0
173.90	95920.0
175.00	7195.0
175.90	91472.0
176.90	6061.0
177.90	225.0
203.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	1198.0
37.00	5278.0
38.00	4420.0
39.00	2422.0
40.00	890.0
40.80	143.0
42.10	113.0
42.90	160.0
44.00	1192.0
45.00	1047.0
46.10	276.0
47.10	1353.0
47.90	625.0
49.00	4605.0
50.00	21640.0
51.00	6536.0
52.00	364.0
53.10	215.0
53.90	222.0
54.90	364.0
56.00	1683.0
57.00	3106.0
57.90	115.0
59.90	1030.0
61.00	5546.0
62.00	5820.0
63.00	4520.0
64.00	932.0
65.00	1626.0
65.90	204.0
67.00	352.0
68.00	11262.0
69.00	11270.0
70.00	732.0
72.00	551.0
73.00	4797.0
74.00	18992.0
75.00	55192.0
76.00	4775.0
77.00	543.0
77.70	589.0
78.90	4008.0
79.90	1089.0
80.90	3854.0
82.00	952.0
85.80	342.0
86.90	5186.0
87.90	4900.0
90.70	402.0
92.00	3434.0
93.00	5047.0
94.00	13764.0
95.00	107728.0
96.00	7165.0
97.10	186.0
104.00	401.0
104.80	184.0
105.90	498.0
106.80	158.0
107.70	102.0
110.80	127.0
114.80	202.0
115.80	378.0
116.80	956.0
117.80	393.0
118.90	865.0
123.80	107.0
127.80	478.0
128.80	182.0
129.80	482.0
130.80	190.0
133.90	127.0
134.90	237.0
136.00	118.0
136.90	223.0
140.00	142.0
140.90	1214.0
141.90	206.0
142.90	1746.0
143.80	185.0
144.90	619.0
145.80	233.0
147.90	223.0
148.80	166.0
150.00	118.0
152.80	132.0
155.00	274.0
155.80	111.0
156.90	307.0
158.70	174.0
160.70	215.0
169.20	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

170.10	176.0
170.90	438.0
171.90	1808.0
173.90	95360.0
175.00	6994.0
175.90	92056.0
176.90	6118.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54