

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
 Data File : VV021974.D
 Acq On : 27 Aug 2021 14:27
 Operator : SY/MD
 Sample : M3549-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV021974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	196774	199101	14.53%	1.874%
2	1.564	156	163	178	rVB	154003	178647	13.04%	1.681%
3	2.108	322	332	344	rBV	311024	453138	33.07%	4.264%
4	2.507	450	456	465	rBV7	1959	2885	0.21%	0.027%
5	2.728	523	525	527	rVV2	453	201	0.01%	0.002%
6	2.761	531	535	540	rBV3	488	468	0.03%	0.004%
7	3.050	623	625	629	rBV3	359	250	0.02%	0.002%
8	3.211	669	675	678	rBV3	214	215	0.02%	0.002%
9	3.278	692	696	697	rBV	277	152	0.01%	0.001%
10	3.310	702	706	711	rBV2	318	286	0.02%	0.003%
11	3.391	728	731	734	rBV	202	156	0.01%	0.001%
12	3.558	780	783	785	rBV	353	187	0.01%	0.002%
13	3.642	807	809	812	rBV	235	143	0.01%	0.001%
14	3.664	812	816	819	rBV2	309	225	0.02%	0.002%
15	3.770	845	849	853	rBV3	452	298	0.02%	0.003%
16	3.876	872	882	918	rBV2	113375	311762	22.75%	2.934%
17	4.352	1014	1030	1060	rBV	210477	529055	38.61%	4.979%
18	4.651	1121	1123	1127	rBV2	381	239	0.02%	0.002%
19	4.674	1127	1130	1132	rBV2	436	308	0.02%	0.003%
20	4.728	1145	1147	1150	rVB	308	147	0.01%	0.001%
21	4.751	1150	1154	1157	rBV2	420	318	0.02%	0.003%
22	4.786	1162	1165	1166	rBV	407	189	0.01%	0.002%
23	4.834	1177	1180	1182	rBV2	256	186	0.01%	0.002%
24	4.944	1211	1214	1218	rVB2	391	216	0.02%	0.002%
25	5.050	1229	1247	1276	rBV2	533282	1370234	100.00%	12.895%
26	5.471	1375	1378	1381	rVB2	551	239	0.02%	0.002%
27	5.619	1412	1424	1456	rBV	418219	835169	60.95%	7.860%
28	5.789	1475	1477	1481	rBV	668	394	0.03%	0.004%
29	5.844	1492	1494	1498	rBV3	426	291	0.02%	0.003%
30	5.912	1504	1515	1532	rBV2	16236	33973	2.48%	0.320%
31	6.072	1551	1565	1590	rBV	298467	610049	44.52%	5.741%
32	6.346	1646	1650	1655	rBV3	447	406	0.03%	0.004%
33	6.497	1694	1697	1700	rVB2	403	259	0.02%	0.002%
34	6.516	1700	1703	1705	rBV2	253	200	0.01%	0.002%
35	6.600	1727	1729	1734	rVB4	515	255	0.02%	0.002%
36	6.625	1734	1737	1739	rBV4	232	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
 Data File : VV021974.D
 Acq On : 27 Aug 2021 14:27
 Operator : SY/MD
 Sample : M3549-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.641	1739	1742	1745	rVV2	321	194	0.01%	0.002%
38	6.715	1761	1765	1768	rVB3	543	355	0.03%	0.003%
39	6.838	1801	1803	1808	rVB2	400	221	0.02%	0.002%
40	6.867	1809	1812	1815	rVV2	314	197	0.01%	0.002%
41	6.915	1824	1827	1831	rVB	213	185	0.01%	0.002%
42	6.989	1839	1850	1876	rBV	165958	304588	22.23%	2.866%
43	7.194	1910	1914	1917	rBV3	477	412	0.03%	0.004%
44	7.320	1940	1953	1971	rBV	655640	1146900	83.70%	10.793%
45	7.625	2038	2048	2072	rBV	111782	198904	14.52%	1.872%
46	7.902	2131	2134	2136	rBV	321	185	0.01%	0.002%
47	7.940	2136	2146	2157	rVB2	2813	5030	0.37%	0.047%
48	7.985	2157	2160	2164	rBV3	464	354	0.03%	0.003%
49	8.030	2172	2174	2179	rVB2	324	215	0.02%	0.002%
50	8.092	2179	2193	2232	rBV	335216	634258	46.29%	5.969%
51	8.442	2300	2302	2304	rBV	271	155	0.01%	0.001%
52	8.622	2351	2358	2362	rBV5	577	806	0.06%	0.008%
53	8.731	2391	2392	2396	rVB2	568	239	0.02%	0.002%
54	8.773	2402	2405	2410	rBV2	183	173	0.01%	0.002%
55	8.799	2410	2413	2416	rVB2	384	223	0.02%	0.002%
56	8.854	2418	2430	2469	rBV	612970	1021129	74.52%	9.610%
57	9.079	2496	2500	2505	rBV4	581	576	0.04%	0.005%
58	9.104	2505	2508	2510	rVV3	813	542	0.04%	0.005%
59	9.146	2514	2521	2531	rBV8	2050	3152	0.23%	0.030%
60	9.320	2572	2575	2579	rBV	291	194	0.01%	0.002%
61	9.355	2584	2586	2591	rVB	334	222	0.02%	0.002%
62	9.426	2605	2608	2610	rBV	201	165	0.01%	0.002%
63	9.477	2622	2624	2627	rBV2	368	176	0.01%	0.002%
64	9.554	2645	2648	2652	rBV2	545	423	0.03%	0.004%
65	9.596	2658	2661	2662	rBV2	311	152	0.01%	0.001%
66	9.709	2694	2696	2701	rVB3	446	285	0.02%	0.003%
67	9.763	2709	2713	2718	rVB4	323	299	0.02%	0.003%
68	9.809	2725	2727	2731	rVB2	341	204	0.01%	0.002%
69	9.841	2735	2737	2740	rVB2	353	167	0.01%	0.002%
70	9.882	2749	2750	2753	rVB2	402	162	0.01%	0.002%
71	9.905	2753	2757	2760	rBV	176	148	0.01%	0.001%
72	9.924	2760	2763	2765	rBV	306	159	0.01%	0.001%
73	10.005	2786	2788	2793	rBV3	238	206	0.02%	0.002%
74	10.098	2815	2817	2819	rBV2	229	136	0.01%	0.001%
75	10.130	2822	2827	2838	rVB4	3055	4517	0.33%	0.043%
76	10.220	2843	2855	2875	rBV	412906	652155	47.59%	6.137%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
 Data File : VV021974.D
 Acq On : 27 Aug 2021 14:27
 Operator : SY/MD
 Sample : M3549-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7A2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.542	2951	2955	2959	rBV3	798	790	0.06%	0.007%
78	10.567	2959	2963	2966	rBV5	718	665	0.05%	0.006%
79	10.706	3001	3006	3009	rBV2	329	247	0.02%	0.002%
80	10.725	3009	3012	3013	rBV3	303	217	0.02%	0.002%
81	10.783	3026	3030	3033	rBV2	560	485	0.04%	0.005%
82	10.924	3064	3074	3080	rBV7	3783	6217	0.45%	0.059%
83	11.069	3117	3119	3122	rVB	349	212	0.02%	0.002%
84	11.091	3122	3126	3134	rBV4	551	613	0.04%	0.006%
85	11.146	3138	3143	3147	rBV3	1295	1527	0.11%	0.014%
86	11.191	3153	3157	3159	rBV2	869	571	0.04%	0.005%
87	11.252	3164	3176	3200	rBV	663707	1046511	76.37%	9.849%
88	11.432	3227	3232	3239	rVB5	2025	2715	0.20%	0.026%
89	11.625	3281	3292	3315	rBV	663569	1052000	76.78%	9.900%
90	11.850	3360	3362	3364	rBV2	942	543	0.04%	0.005%
91	11.995	3403	3407	3410	rBV3	489	408	0.03%	0.004%
92	12.085	3432	3435	3436	rBV2	520	303	0.02%	0.003%
93	12.191	3465	3468	3473	rVB2	660	385	0.03%	0.004%
94	12.516	3566	3569	3571	rBV	470	209	0.02%	0.002%
95	12.593	3589	3593	3596	rBV2	525	527	0.04%	0.005%
96	12.651	3607	3611	3617	rBV3	619	791	0.06%	0.007%
97	12.860	3673	3676	3677	rBV	237	146	0.01%	0.001%
98	12.995	3716	3718	3722	rBV2	339	286	0.02%	0.003%
99	13.043	3730	3733	3735	rBV2	401	214	0.02%	0.002%
100	13.959	4016	4018	4019	rBV	388	161	0.01%	0.002%




Sum of corrected areas: 10625887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
Data File : VV021974.D
Acq On : 27 Aug 2021 14:27
Operator : SY/MD
Sample : M3549-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

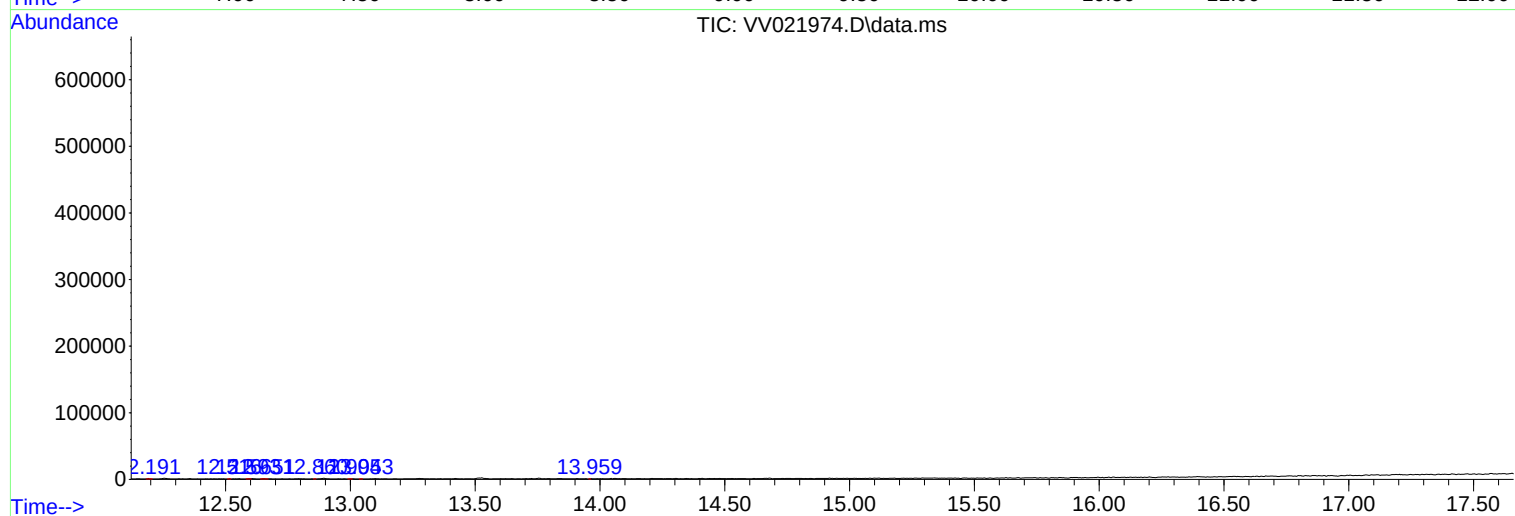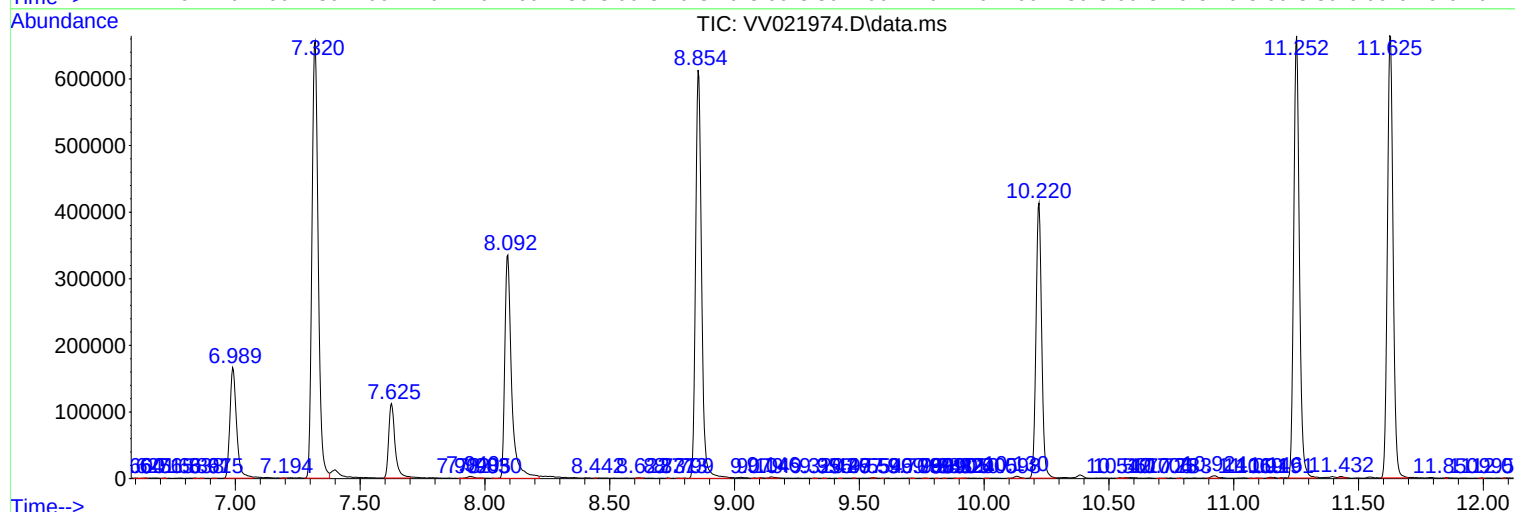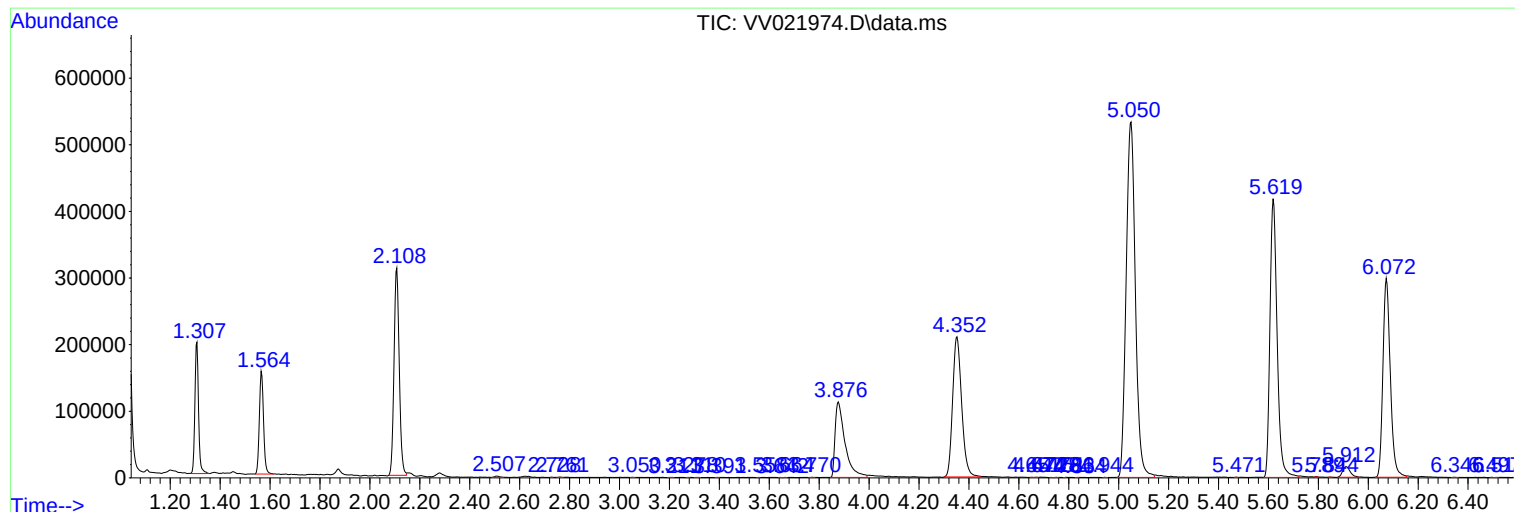

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
Data File : VV021974.D
Acq On : 27 Aug 2021 14:27
Operator : SY/MD
Sample : M3549-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
Data File : VV021974.D
Acq On : 27 Aug 2021 14:27
Operator : SY/MD
Sample : M3549-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7A2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------