


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082721\
Data File : VV021962.D
Acq On : 27 Aug 2021 08:49
Operator : SY/MD
Sample : BFB223
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB223

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Title : VOC Analysis
Last Update : Sat Aug 28 02:34:14 2021

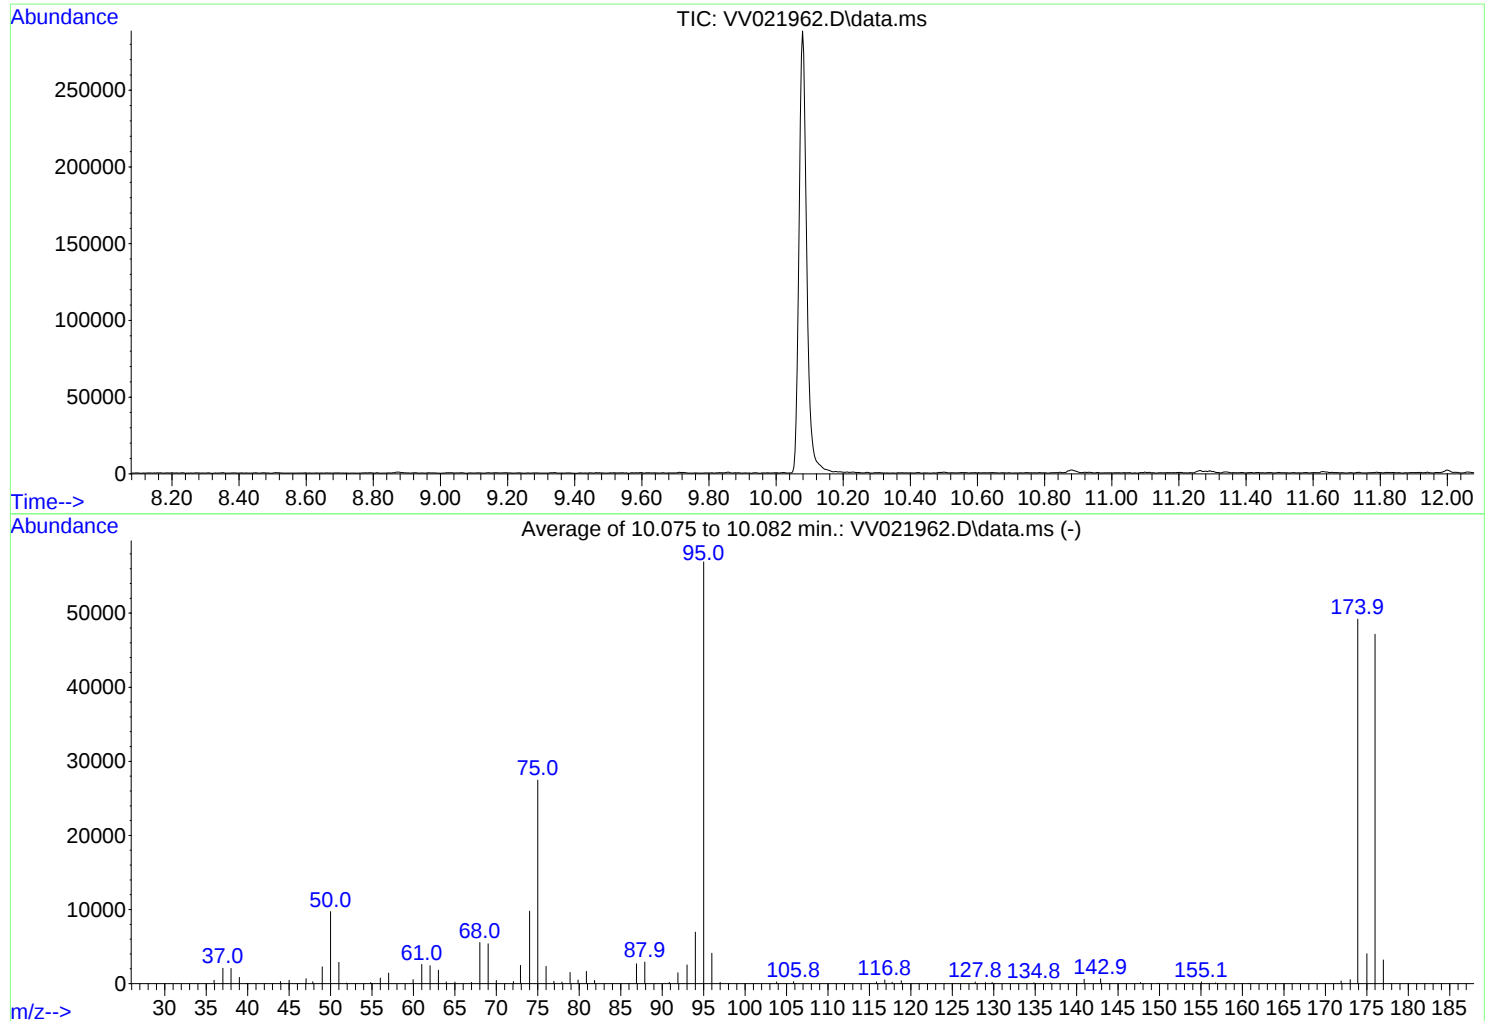

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	9719	PASS
75	95	30	80	48.2	27456	PASS
95	95	100	100	100.0	56923	PASS
96	95	5	9	7.2	4110	PASS
173	174	0.00	2	1.1	532	PASS
174	95	50	120	86.4	49184	PASS
175	174	5	9	8.2	4036	PASS
176	174	95	105	95.9	47165	PASS
177	176	5	10	6.8	3203	PASS

m/z	Abundance
35.90	478.0
37.00	2009.0
38.00	1938.0
39.00	833.0
40.00	246.0
44.00	771.0
45.00	408.0
47.00	579.0
47.80	247.0
49.00	2129.0
50.00	9148.0
51.00	2738.0
54.90	154.0
56.00	683.0
57.00	1462.0
60.00	555.0
61.00	2463.0
62.00	2373.0
63.00	1870.0
64.00	244.0
65.00	229.0
67.00	174.0
68.00	5125.0
69.00	5380.0
70.00	399.0
72.00	317.0
72.90	2336.0
74.00	9712.0
75.00	26776.0
76.00	2264.0
76.90	290.0
77.90	251.0
78.90	1508.0
79.90	498.0
80.80	1591.0
81.90	405.0
86.00	108.0
86.90	2719.0
87.90	2712.0
90.90	150.0
91.90	1401.0
93.00	2431.0
94.00	7007.0
95.00	55912.0
96.00	4015.0
97.00	155.0
103.80	243.0
105.90	288.0
115.80	252.0
116.90	447.0
117.70	229.0
118.90	378.0
127.70	230.0
129.00	167.0
129.80	171.0
134.90	118.0
136.80	131.0
140.90	554.0
142.90	627.0
147.70	154.0
155.00	257.0
156.70	106.0
171.90	346.0
173.00	562.0
173.90	49736.0
175.00	4056.0
176.00	46768.0
177.00	3188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

Scan 2800 (10.043 min): VV021962.D\data.ms
BFB223

m/z	Abundance
39.90	237.0
43.90	440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
36.00	409.0
37.00	2079.0
38.00	2109.0
39.00	845.0
39.90	249.0
44.00	669.0
45.00	469.0
47.10	764.0
47.90	255.0
49.00	2324.0
50.00	9961.0
51.00	2923.0
51.90	132.0
54.80	166.0
56.00	809.0
57.00	1335.0
59.90	508.0
61.00	2592.0
62.00	2428.0
63.00	1715.0
63.90	245.0
65.00	200.0
67.00	170.0
68.00	5728.0
69.00	5172.0
70.00	485.0
72.00	239.0
72.90	2544.0
74.00	9329.0
75.00	27160.0
76.00	2342.0
77.00	359.0
77.90	184.0
78.90	1506.0
79.80	510.0
80.90	1681.0
81.80	420.0
86.90	2459.0
87.90	2961.0
90.90	193.0
91.90	1496.0
93.00	2546.0
94.00	6654.0
95.00	56064.0
96.00	4009.0
97.00	173.0
103.80	229.0
105.80	246.0
115.90	237.0
116.80	547.0
117.80	183.0
118.80	381.0
127.80	208.0
129.00	106.0
129.80	193.0
134.80	129.0
140.90	649.0
142.90	634.0
147.70	158.0
149.80	117.0
155.00	194.0
156.80	108.0
160.80	112.0
171.90	378.0
173.00	476.0
173.90	46688.0
175.00	3866.0
176.00	45792.0
177.00	3088.0
177.90	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223

m/z	Abundance
36.00	470.0
37.00	2155.0
38.00	2116.0
39.00	826.0
40.00	244.0
44.00	738.0
45.00	479.0
47.10	690.0
47.90	259.0
49.00	2367.0
50.00	10049.0
51.00	2974.0
51.90	121.0
54.90	166.0
56.00	803.0
57.00	1515.0
59.90	559.0
61.00	2704.0
62.00	2484.0
63.00	1874.0
63.90	246.0
65.00	229.0
67.00	178.0
68.00	5769.0
69.00	5572.0
70.00	446.0
72.10	278.0
72.90	2534.0
74.00	10284.0
75.00	28432.0
76.00	2420.0
76.90	345.0
77.90	237.0
78.90	1540.0
79.90	507.0
80.90	1693.0
81.80	442.0
86.90	2846.0
87.90	3054.0
90.80	181.0
91.90	1505.0
93.00	2588.0
94.00	7221.0
95.00	58792.0
96.00	4307.0
97.00	184.0
103.80	233.0
105.90	292.0
115.80	236.0
116.80	516.0
117.70	196.0
118.90	411.0
127.70	260.0
129.00	159.0
129.80	182.0
134.80	125.0
136.90	113.0
140.90	607.0
142.90	690.0
147.70	172.0
149.80	109.0
155.10	235.0
156.70	124.0
171.90	388.0
173.00	558.0
173.90	51128.0
175.00	4187.0
176.00	48936.0
177.00	3333.0

Instrument :
MSVOA_V
ClientSampleId :
BFB223