

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
 Data File : VV007242.D
 Acq On : 29 Aug 2018 00:30
 Operator : SY/MD
 Sample : J4647-09MS
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAB74MS

Quant Time: Aug 29 04:03:31 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 04:00:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	230305	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	231711	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	88836	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71887	4.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.00%
7) Chloroethane-d5	1.58	69	64730	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.13	63	140806	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	99.60%
20) 2-Butanone-d5	3.97	46	216138	52.95	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.90%
24) Chloroform-d	4.40	84	157884	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.09	65	81856	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.10	84	292921	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
36) 1,2-Dichloropropane-d6	6.12	67	101735	4.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.00%
41) Toluene-d8	7.37	98	217507	3.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.00%
43) trans-1,3-Dichloropropene-	7.67	79	31625	4.16	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.20%
46) 2-Hexanone-d5	8.15	63	87063	43.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.00%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	77320	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	80299	4.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.00%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) 1,1-Dichloroethene	2.14	96	86917	6.237	ug/L	88
13) Acetone	2.21	43	10083	4.926	ug/L	99
21) 2-Butanone	4.07	43	2577	0.605	ug/L	94
33) Benzene	5.15	78	396921	5.783	ug/L	100
34) Trichloroethene	5.96	95	96111	5.551	ug/L	99
35) Methylcyclohexane	6.12	83	25271	0.998	ug/L #	17
37) 1,2-Dichloropropane	6.12	63	10525	0.578	ug/L #	85
42) Toluene	7.44	91	373311	5.539	ug/L	98
47) Tetrachloroethene	8.02	164	10332	0.722	ug/L	92
48) 2-Hexanone	8.20	43	42627	5.986	ug/L	90
49) Dibromochloromethane	8.02	129	8922	0.604	ug/L #	10
51) Chlorobenzene	8.93	112	243334	5.311	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082818\
Data File : VV007242.D
Acq On : 29 Aug 2018 00:30
Operator : SY/MD
Sample : J4647-09MS
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAB74MS

Quant Time: Aug 29 04:03:31 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 04:00:48 2018
Response via : Initial Calibration

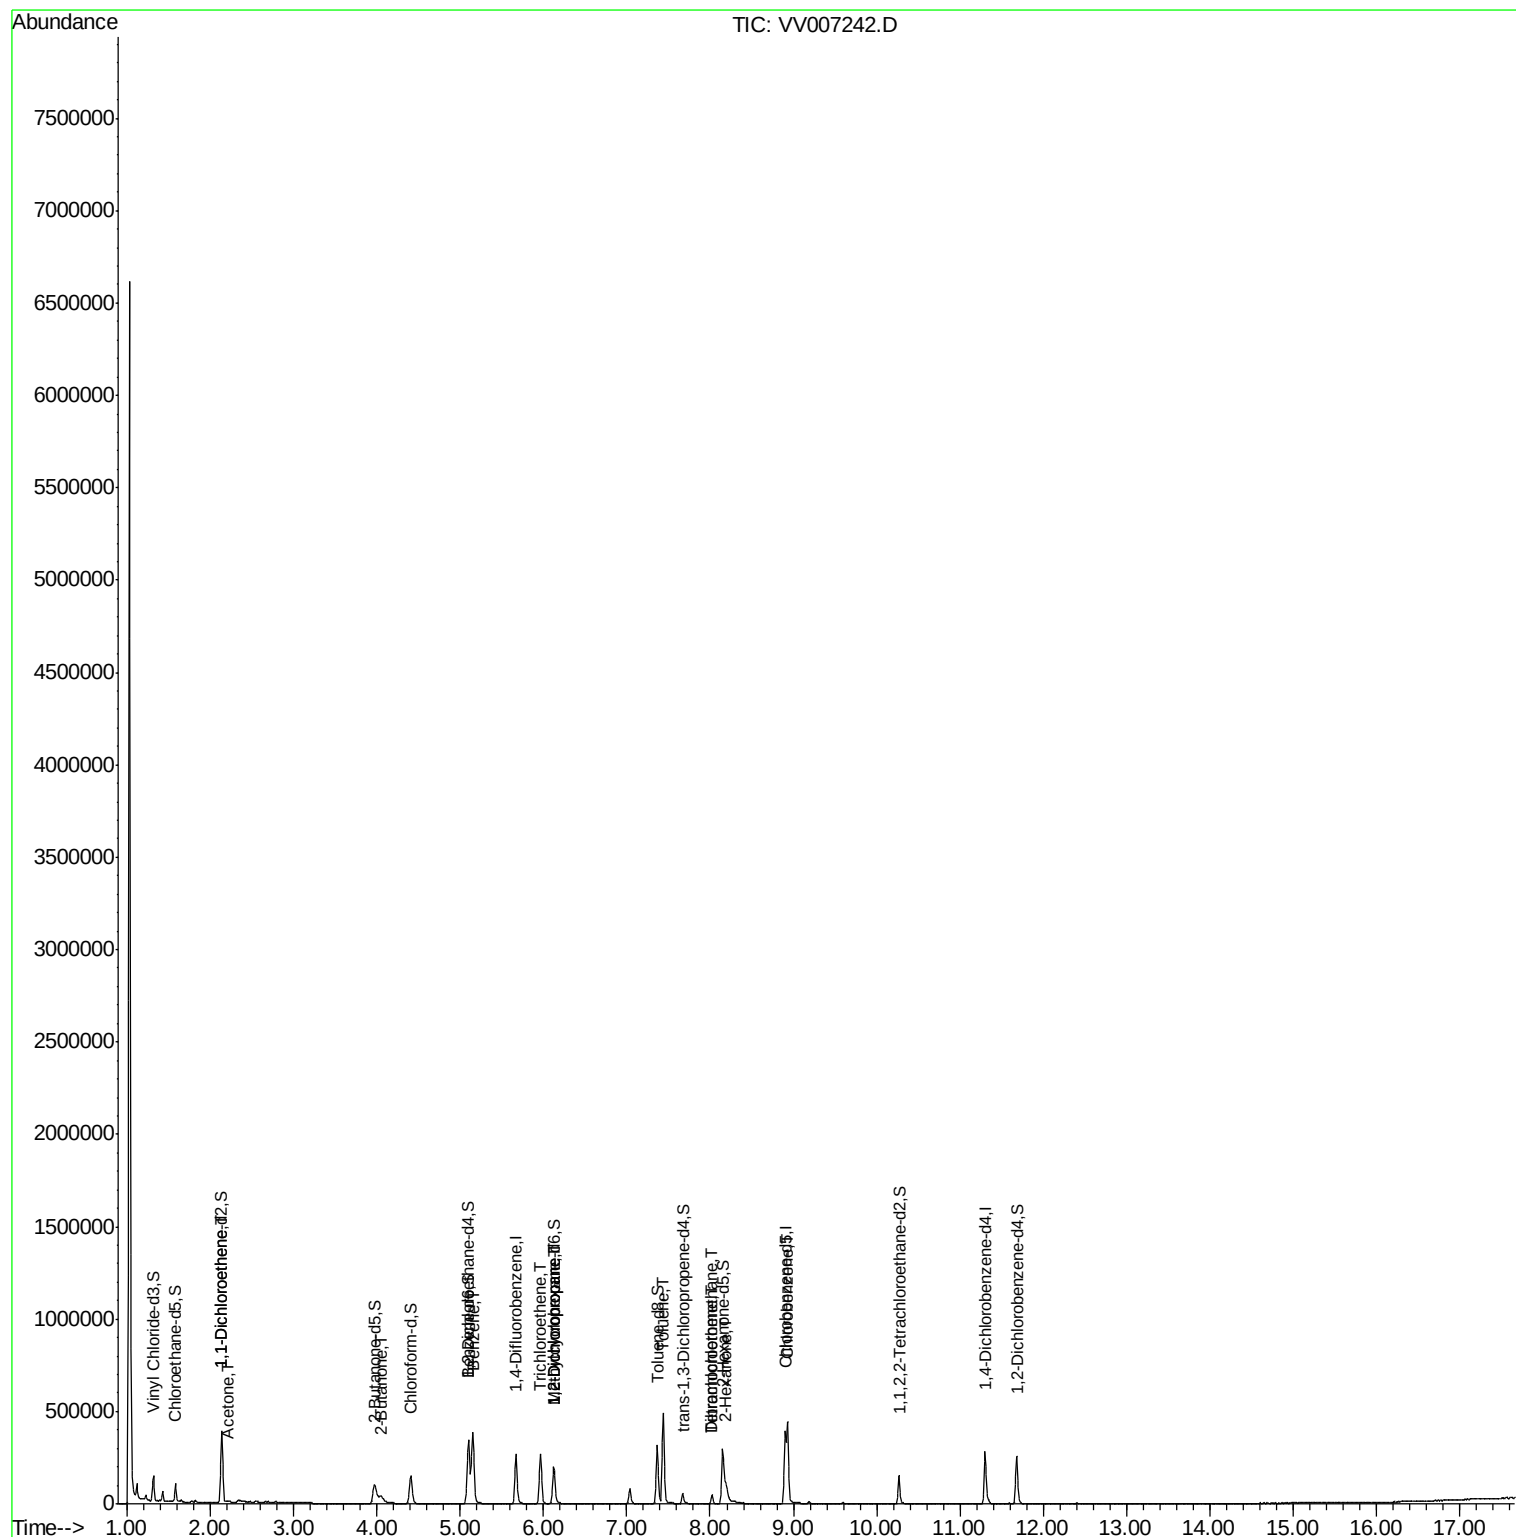



#12

1,1-Dichloroethene

Concen: 6.237 ug/L

RT: 2.14 min Scan# 390

Delta R.T. 0.00 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30

Instrument :

MSVOA_V

ClientSampleId :

GAB74MS


Tot Ion: 96 Resp: 86917

Ion Ratio Lower Upper

96 100

61 149.9 112.3 208.5




63 88.7 75.4 140.0

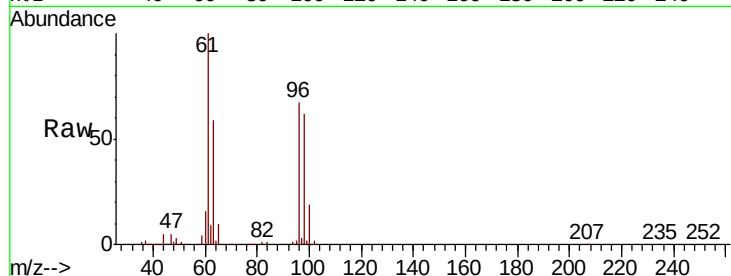

Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 63.00 (62.70 to 63.70): VV0

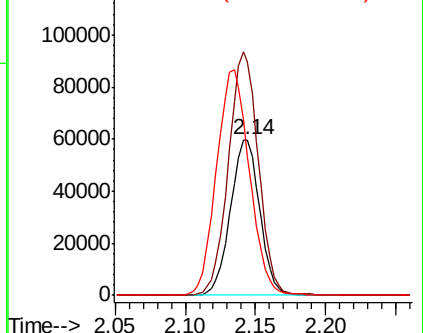

#13

Acetone

Concen: 4.926 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.01 min

Lab File: VV007242.D


Acq: 29 Aug 2018 00:30

Tgt Ion: 43 Resp: 10083

Ion Ratio Lower Upper



43 100


58 34.8 0.0 70.2



Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

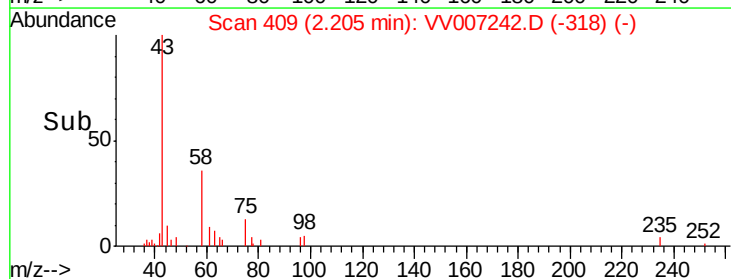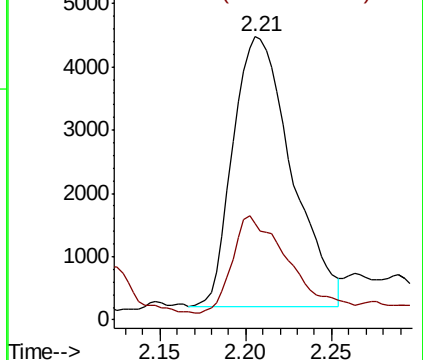



#21

2-Butanone

Concen: 0.605 ug/L

RT: 4.07 min Scan# 988

Delta R.T. 0.01 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30

Instrument :

MSVOA_V

ClientSampleId :





GAB74MS

Tot Ion: 43 Resp: 2577

Ion Ratio Lower Upper

43 100

72 27.9 12.4 37.0

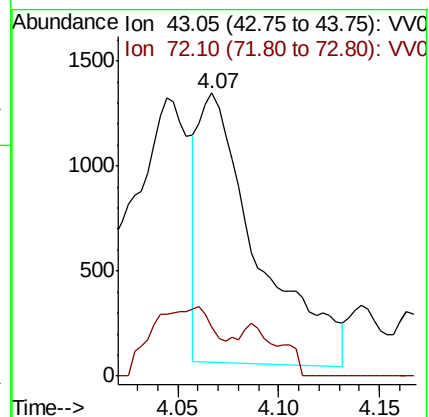

#33

Benzene

Concen: 5.783 ug/L




RT: 5.15 min Scan# 1325


Delta R.T. 0.00 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30

Tgt Ion: 78 Resp: 396921

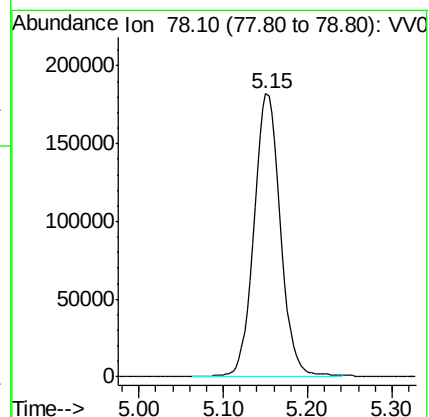



#34

Trichloroethene

Concen: 5.551 ug/L

RT: 5.96 min Scan# 1578

Delta R.T. 0.00 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30

Instrument :

MSVOA_V

ClientSampleId :

GAB74MS

Tot Ion: 95 Resp: 96111


Ion Ratio Lower Upper

95 100

97 64.2 44.2 82.2

132 100.3 71.3 132.3

130 104.3 72.8 135.2






Abundance Ion 95.00 (94.70 to 95.70): VV007230.D (-1562) (-)

Ion 96.95 (96.65 to 97.65): VV007230.D (-1562) (-)

Ion 131.95 (131.65 to 132.65): VV007230.D (-1562) (-)

Ion 129.95 (129.65 to 130.65): VV007230.D (-1562) (-)

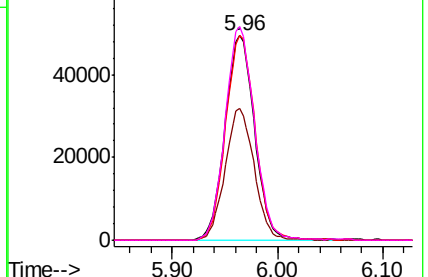

#35

Methylcyclohexane

Concen: 0.998 ug/L

RT: 6.12 min Scan# 1628

Delta R.T. -0.05 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30


Tgt Ion: 83 Resp: 25271

Ion Ratio Lower Upper

83 100

55 0.6 64.0 96.0#



98 0.7 38.8 58.2#




Abundance Ion 83.15 (82.85 to 83.85): VV007230.D (-1634) (-)

Ion 55.10 (54.80 to 55.80): VV007230.D (-1634) (-)

Ion 98.15 (97.85 to 98.85): VV007230.D (-1634) (-)



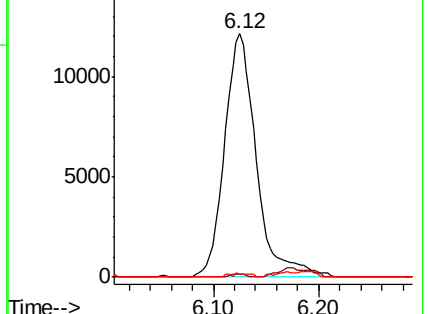





#37
 1,2-Dichloropropane
 Concen: 0.578 ug/L
 RT: 6.12 min Scan# 1628
 Delta R.T. -0.10 min
 Lab File: VV007242.D
 Acq: 29 Aug 2018 00:30




Instrument :
 MSVOA_V
 ClientSampleId :
 GAB74MS


Tot Ion: 63 Resp: 10525
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.9 5.9#

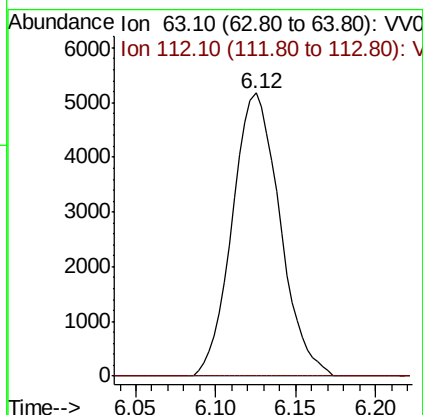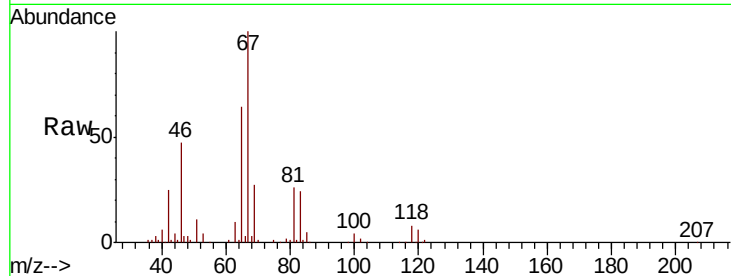

#42
 Toluene
 Concen: 5.539 ug/L
 RT: 7.44 min Scan# 2036
 Delta R.T. 0.00 min
 Lab File: VV007242.D
 Acq: 29 Aug 2018 00:30

Tgt Ion: 91 Resp: 373311
 Ion Ratio Lower Upper
 91 100
 92 57.4 41.1 76.3



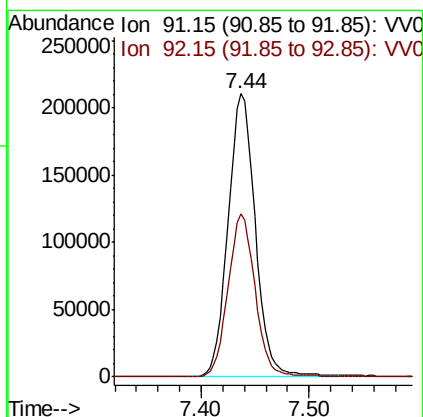
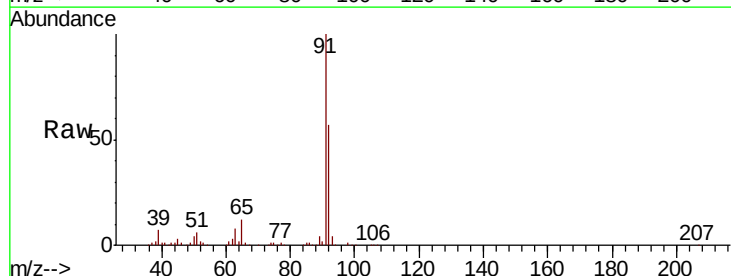


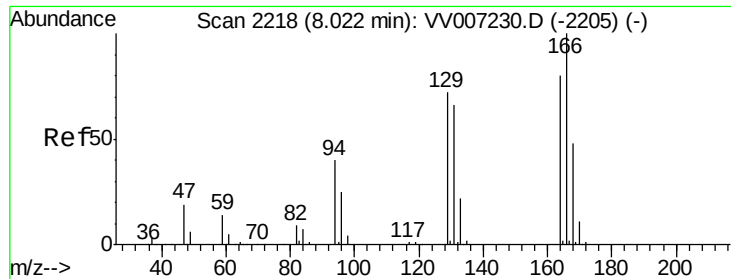

#47
Tetrachloroethene
Concen: 0.722 ug/L
RT: 8.02 min Scan# 2218
Delta R.T. 0.00 min
Lab File: VV007242.D
Acq: 29 Aug 2018 00:30




Instrument :
MSVOA_V
ClientSampleId :
GAB74MS


Tot Ion:164	Resp:	10332
Ion Ratio	Lower	Upper
164 100		
129 88.3	62.7	116.5
131 91.7	60.1	111.7
166 138.4	86.4	160.4

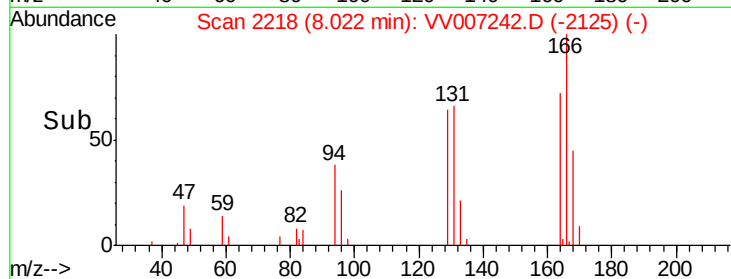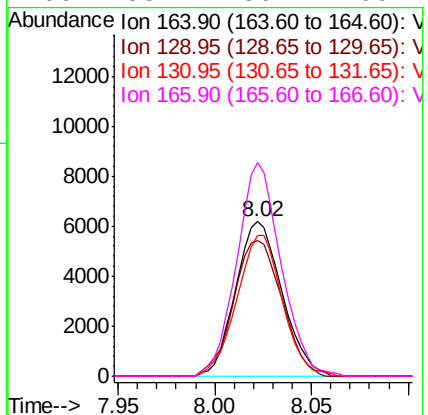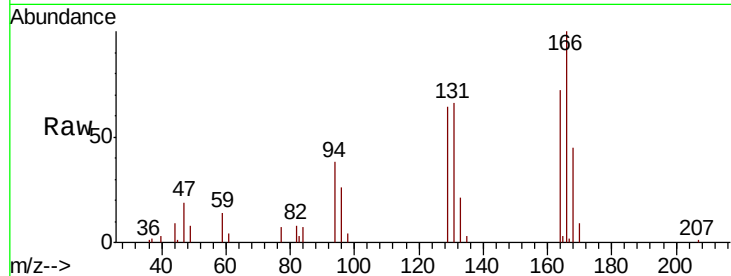

#48
2-Hexanone
Concen: 5.986 ug/L
RT: 8.20 min Scan# 2273
Delta R.T. 0.00 min
Lab File: VV007242.D
Acq: 29 Aug 2018 00:30

Tgt	Ion: 43	Resp:	42627
Ion	Ratio	Lower	Upper
43	100		
58	53.0	50.0	75.0
57	18.9	16.6	25.0
100	10.9	10.2	15.4

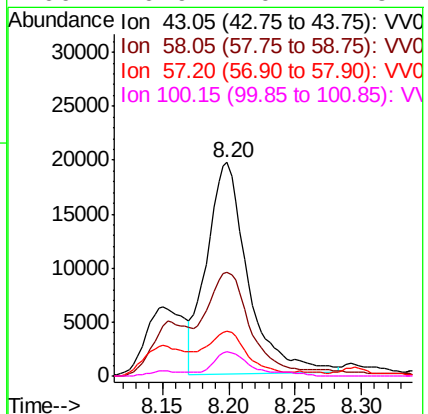



#49

Dibromochloromethane

Concen: 0.604 ug/L

RT: 8.02 min Scan# 2218

Delta R.T. -0.27 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30

Instrument :

MSVOA_V

ClientSampleId :


GAB74MS

Tot Ion:129 Resp: 8922

Ion Ratio Lower Upper




129 100

127 0.0 54.9 101.9#

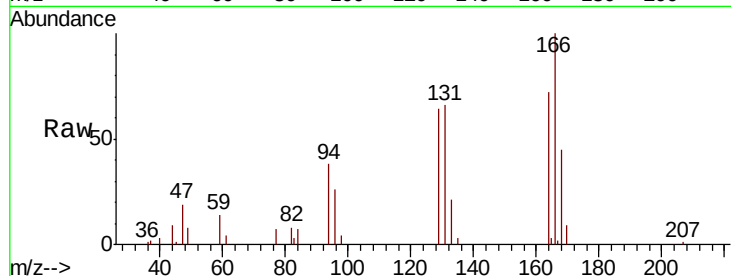

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

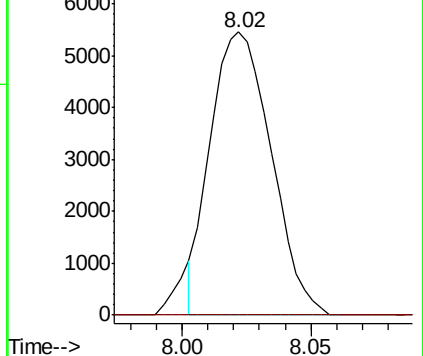

#51

Chlorobenzene

Concen: 5.311 ug/L

RT: 8.93 min Scan# 2501

Delta R.T. 0.00 min

Lab File: VV007242.D

Acq: 29 Aug 2018 00:30


Tgt Ion:112 Resp: 243334

Ion Ratio Lower Upper

112 100

114 31.2 22.0 41.0

77 55.5 45.9 68.9



Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VV0

