

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
 Data File : VV007234.D
 Acq On : 28 Aug 2018 20:53
 Operator : SY/MD
 Sample : J4628-19
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB3G4

Quant Time: Aug 29 04:23:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 04:00:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	220886	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	222619	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	87188	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72333	4.61	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.20%
7) Chloroethane-d5	1.58	69	61571	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.13	63	96570	3.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.20%
20) 2-Butanone-d5	3.97	46	204423	52.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.44%
24) Chloroform-d	4.40	84	149615	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.09	65	75719	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.10	84	285318	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
36) 1,2-Dichloropropane-d6	6.12	67	96083	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.37	98	207528	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.40%
43) trans-1,3-Dichloropropene-	7.67	79	28129	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	8.15	63	64834	33.71	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.42%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	70900	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	79848	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	11795	6.01 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
Data File : VV007234.D
Acq On : 28 Aug 2018 20:53
Operator : SY/MD
Sample : J4628-19
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB3G4

Quant Time: Aug 29 04:23:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 04:00:48 2018
Response via : Initial Calibration

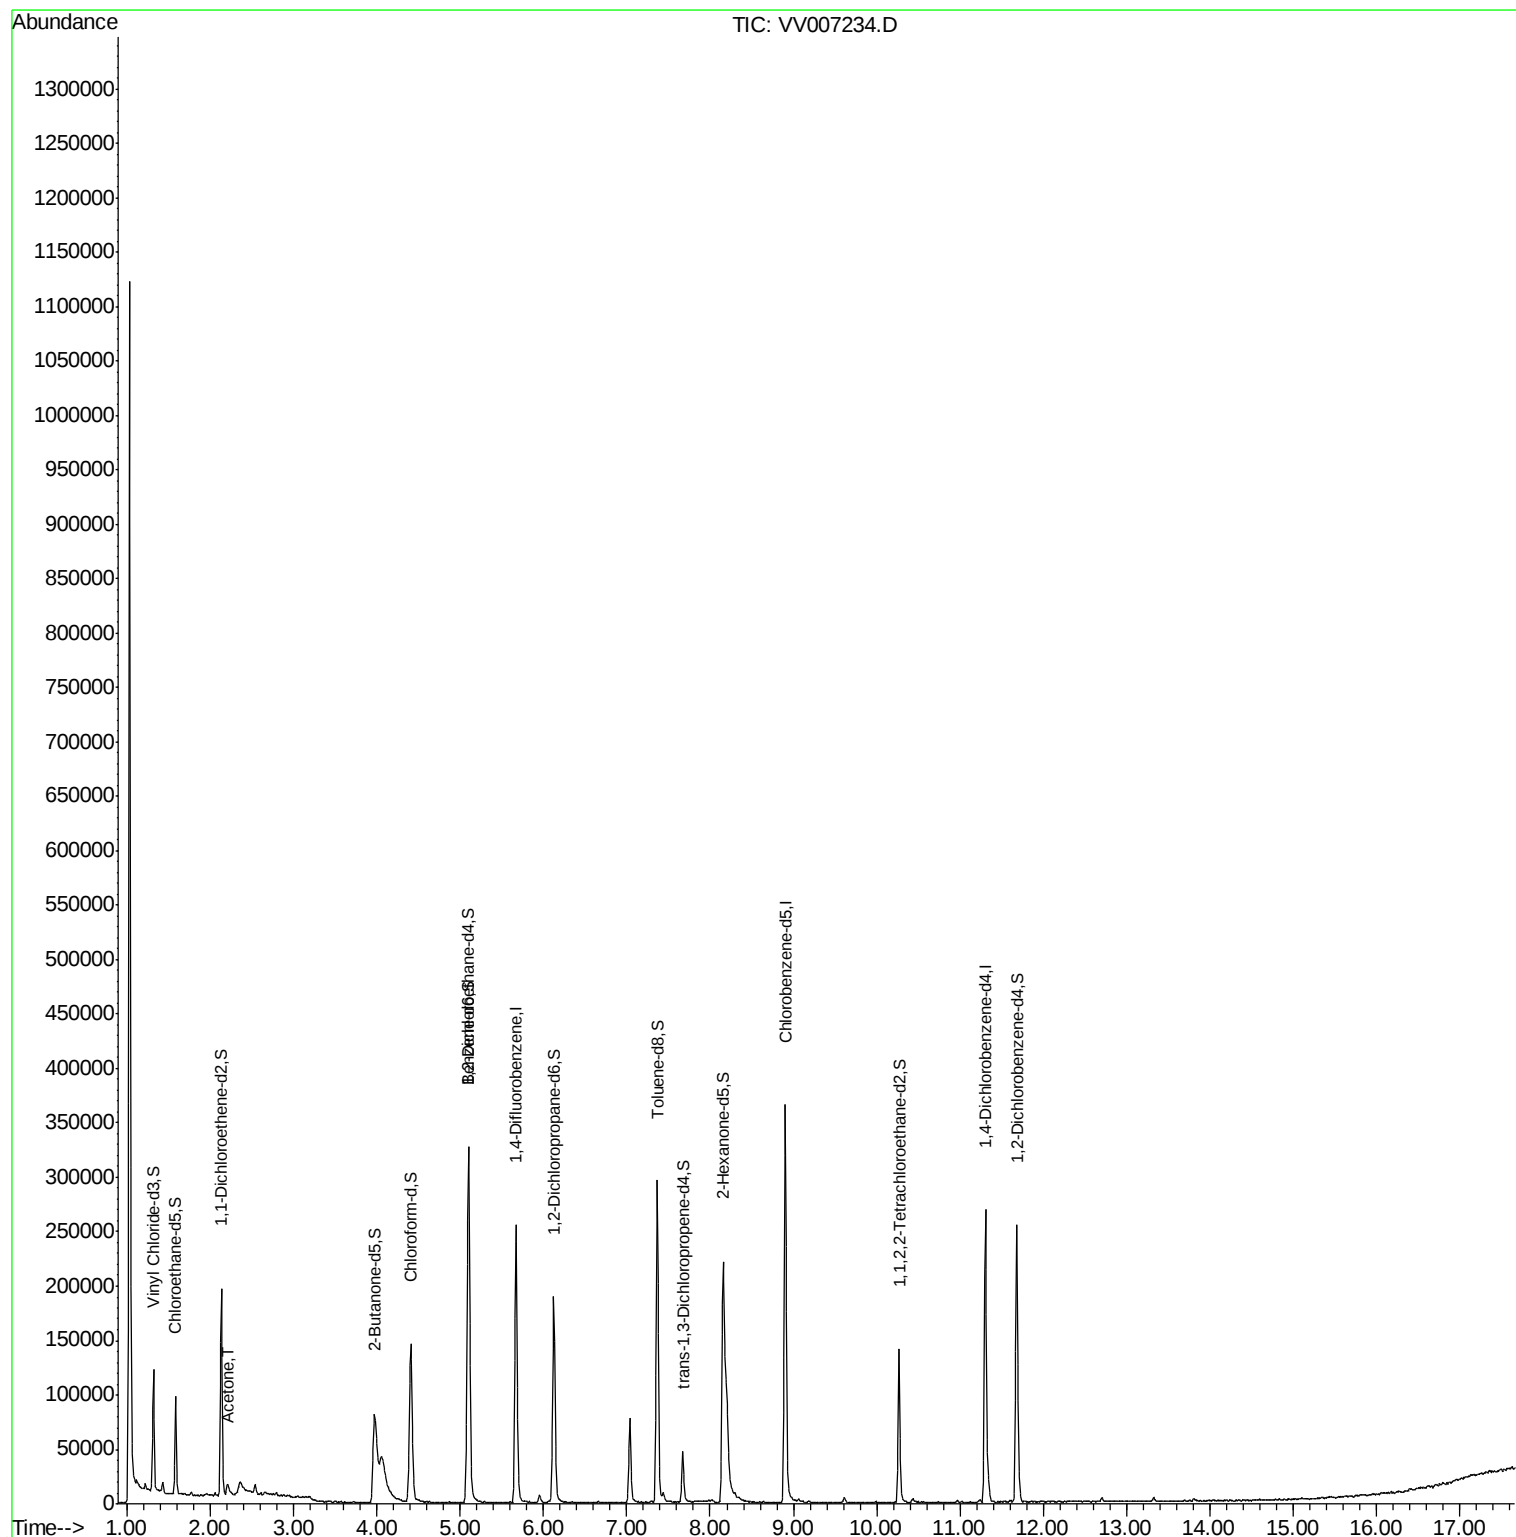

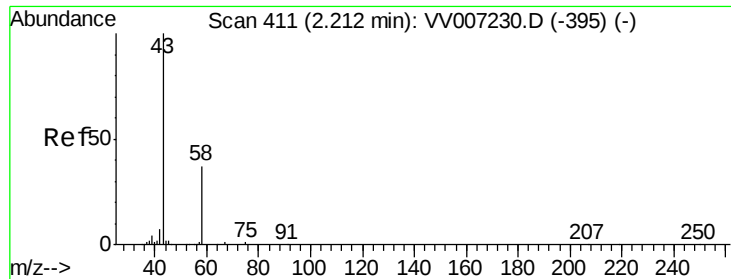

#13

Acetone

Concen: 6.01 ug/L

RT: 2.21 min Scan# 411

Delta R.T. 0.00 min

Lab File: VV007234.D

Acq: 28 Aug 2018 20:53

Instrument :
MSVOA_V
ClientSampleId :
DB3G4

Tot Ion: 43 Resp: 11795

Ion Ratio Lower Upper

43 100

58 40.3 0.0 70.2

